

SUPERVISOR TEST




WARREN COUNTY
SHERRIF'S OFFICE
DATAMASTER dmt: 144506

Date: 09/19/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18170

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:32
INTERNAL STANDARD	VERIFIED	05:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:33
BLANK TEST	0.00	05:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:34
BLANK TEST	0.00	05:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:35
BLANK TEST	0.00	05:36

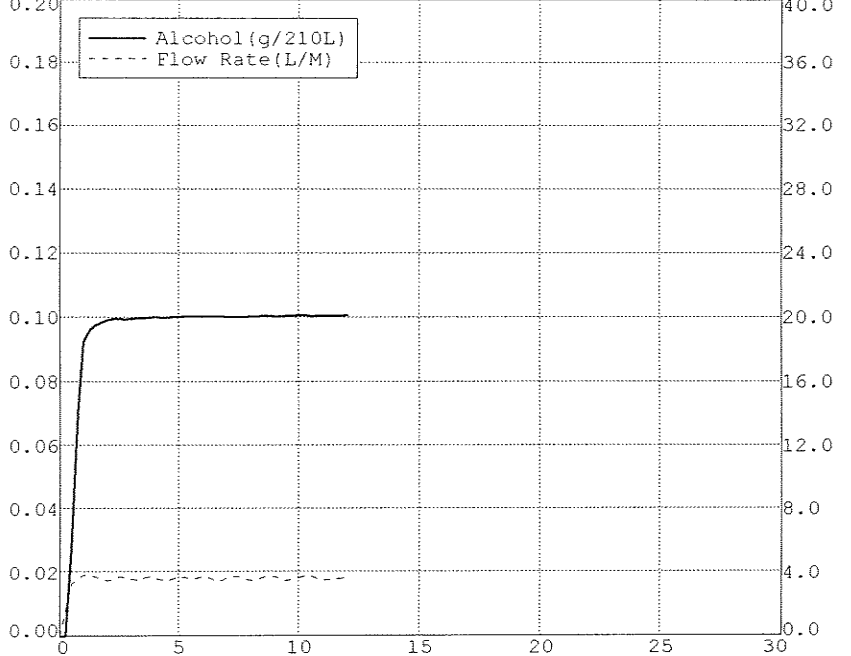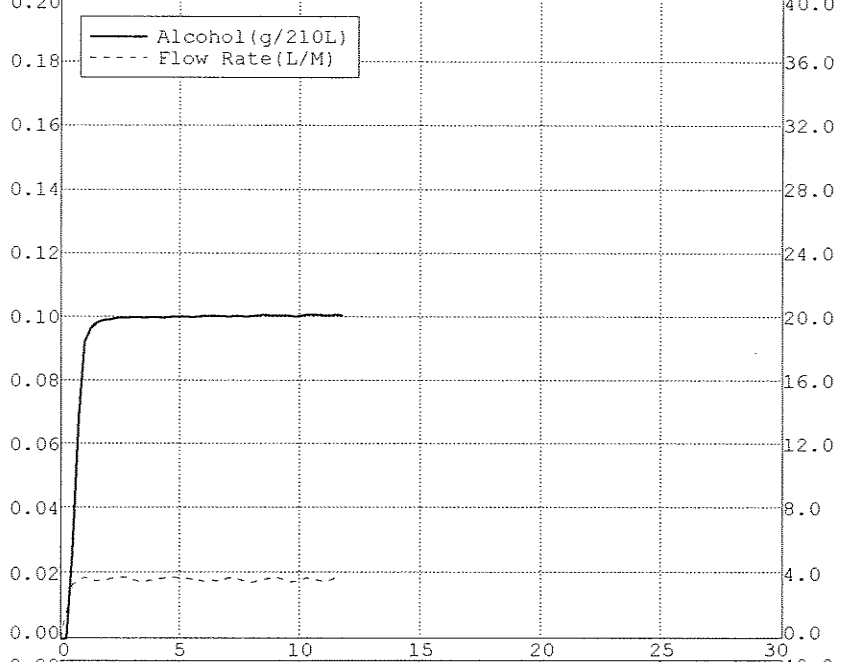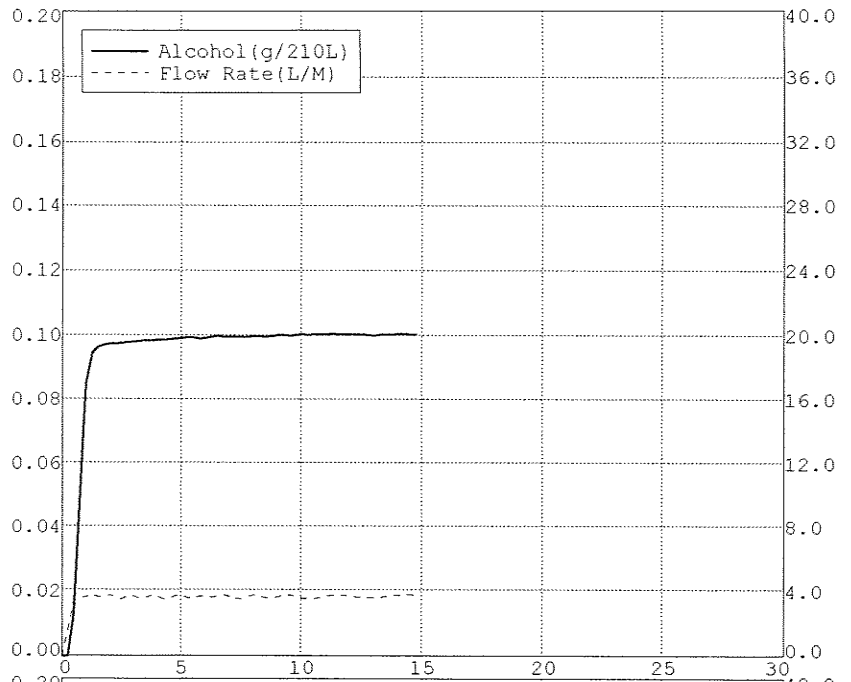

Charles B. Geisler #22