

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 09/22/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18170

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:28
INTERNAL STANDARD	VERIFIED	02:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:28
BLANK TEST	0.00	02:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:30
BLANK TEST	0.00	02:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:31
BLANK TEST	0.00	02:32

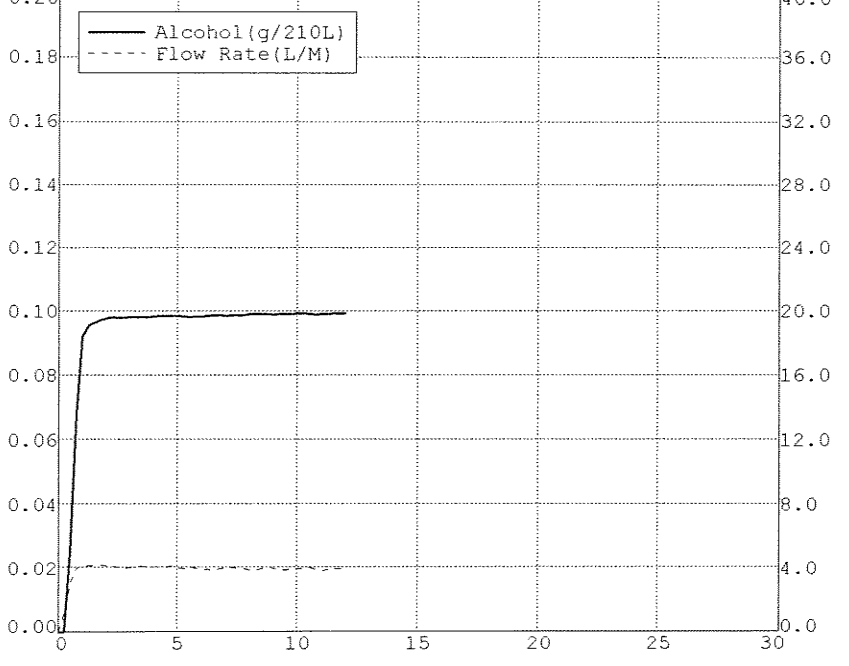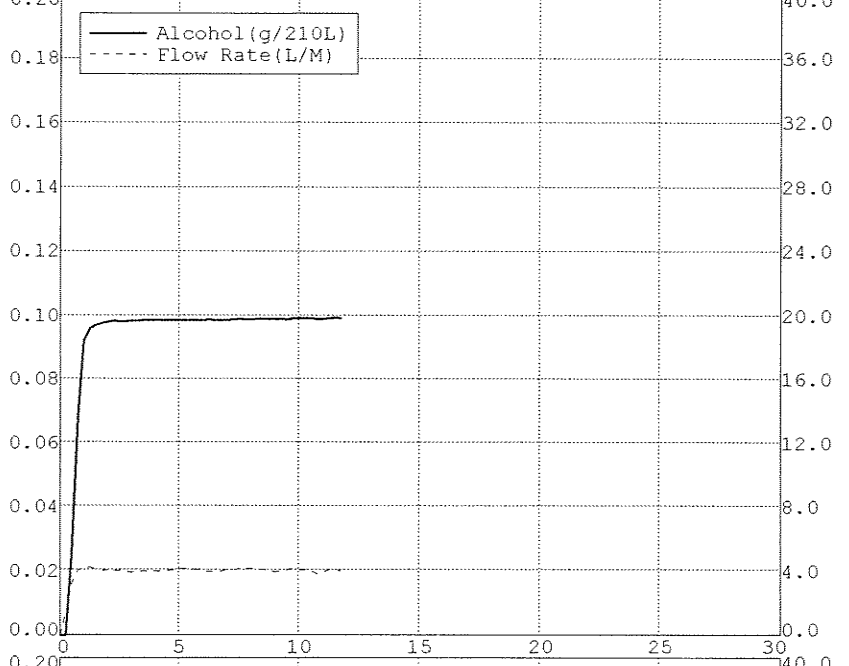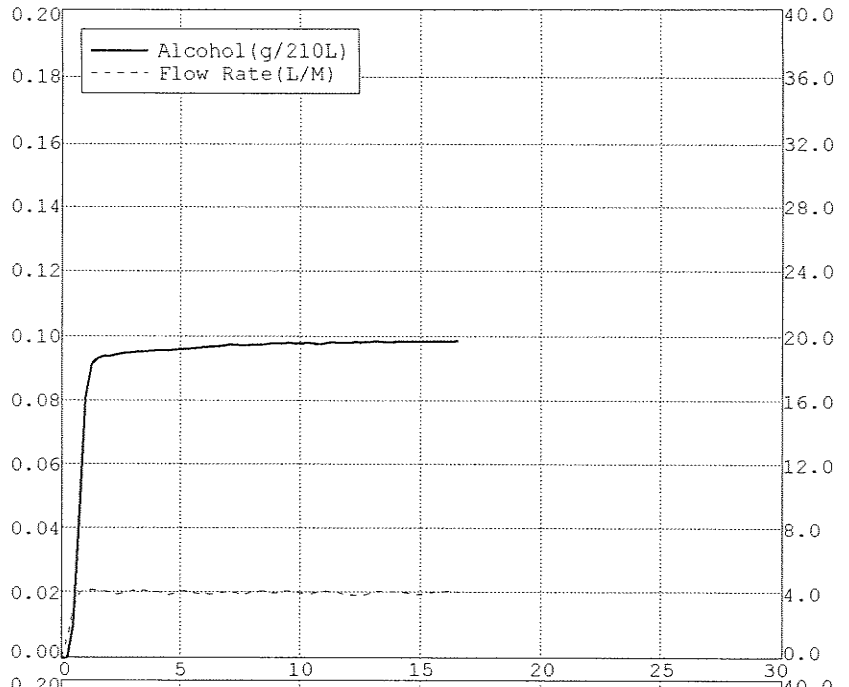

Charles B Geisler