

SOLUTION CHANGE




 WARREN COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 144506

Date: 11/01/2018

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:09
INTERNAL STANDARD	VERIFIED	12:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:10
BLANK TEST	0.00	12:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:11
BLANK TEST	0.00	12:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:12
BLANK TEST	0.00	12:13

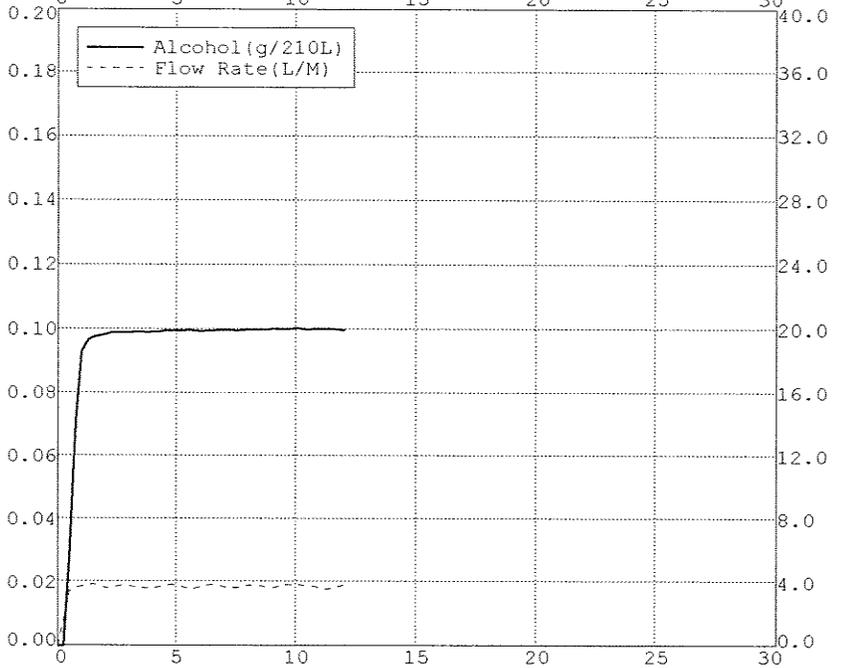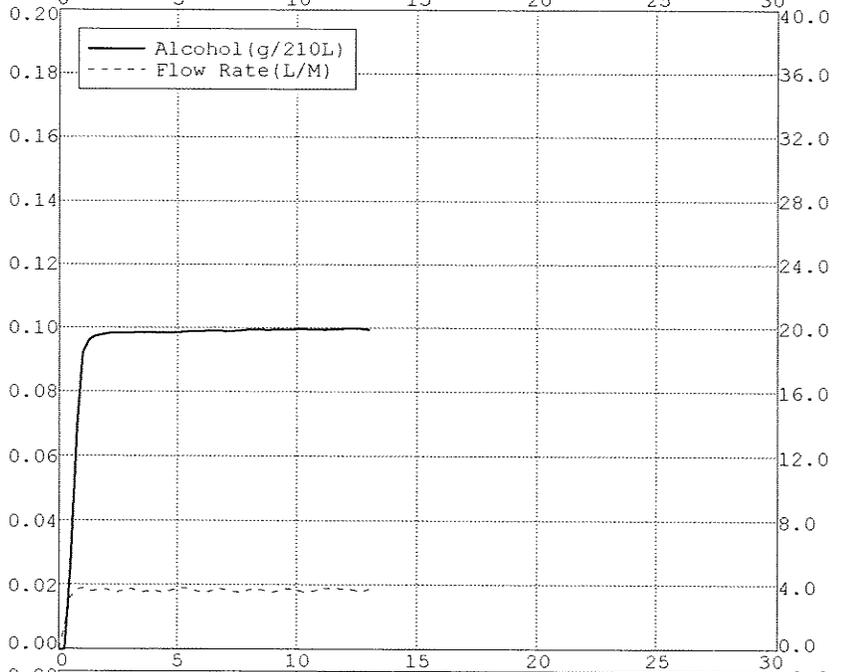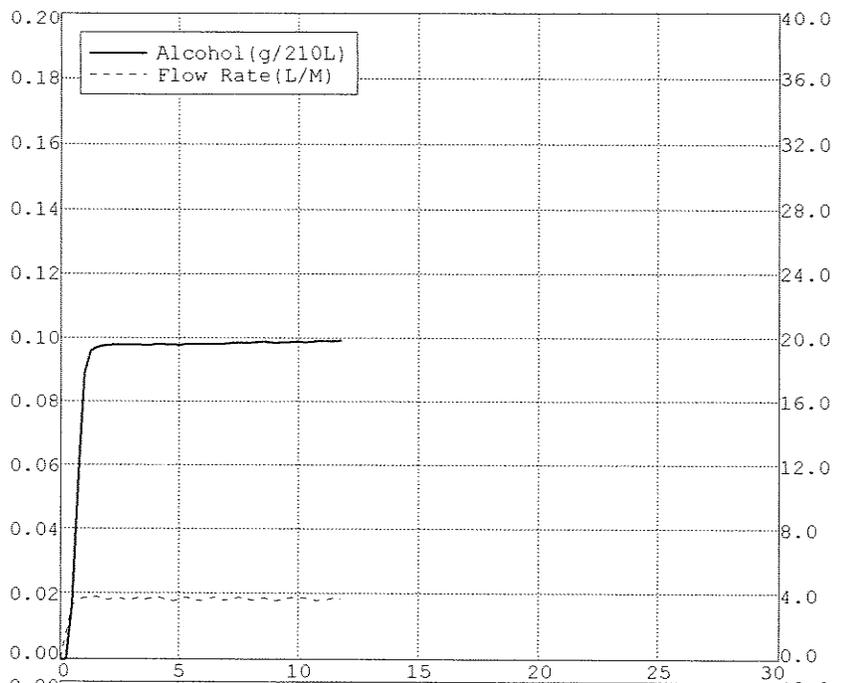

Charles B. Geisler #241