

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 11/14/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:59
INTERNAL STANDARD	VERIFIED	04:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:00
BLANK TEST	0.00	05:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:01
BLANK TEST	0.00	05:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:02
BLANK TEST	0.00	05:03

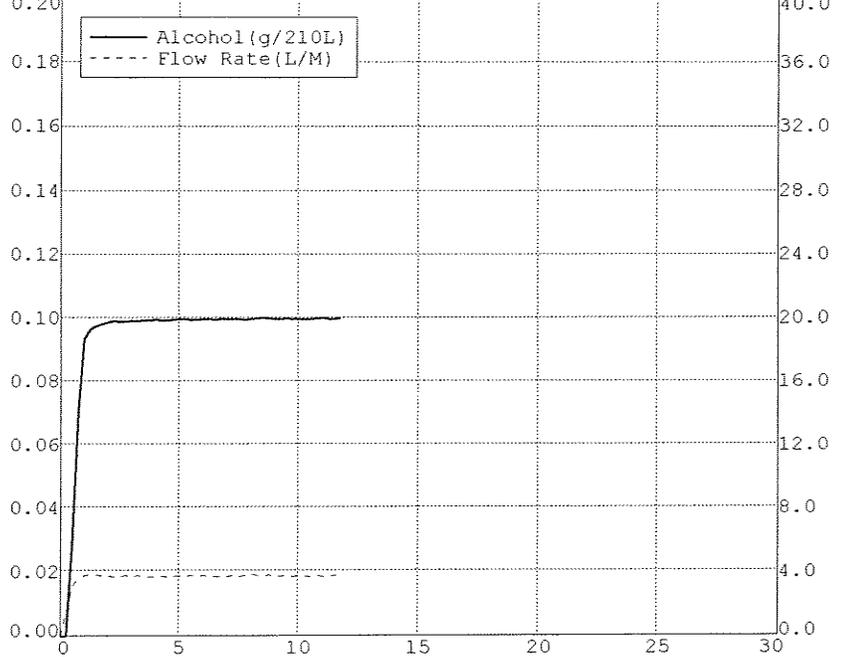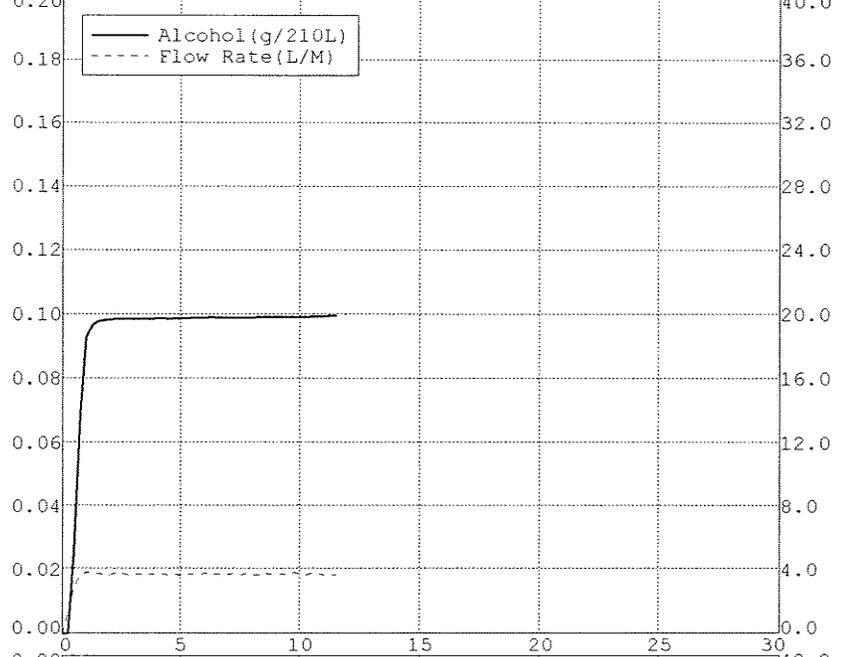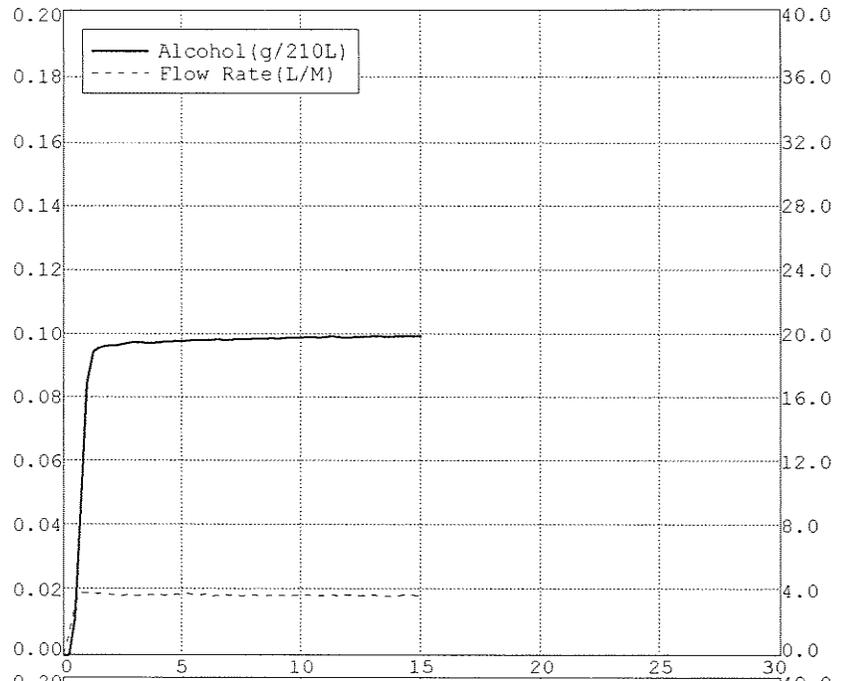

Charles B. Geisler #200