

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 11/27/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:36
INTERNAL STANDARD	VERIFIED	05:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:37
BLANK TEST	0.00	05:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:38
BLANK TEST	0.00	05:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	05:39
BLANK TEST	0.00	05:40

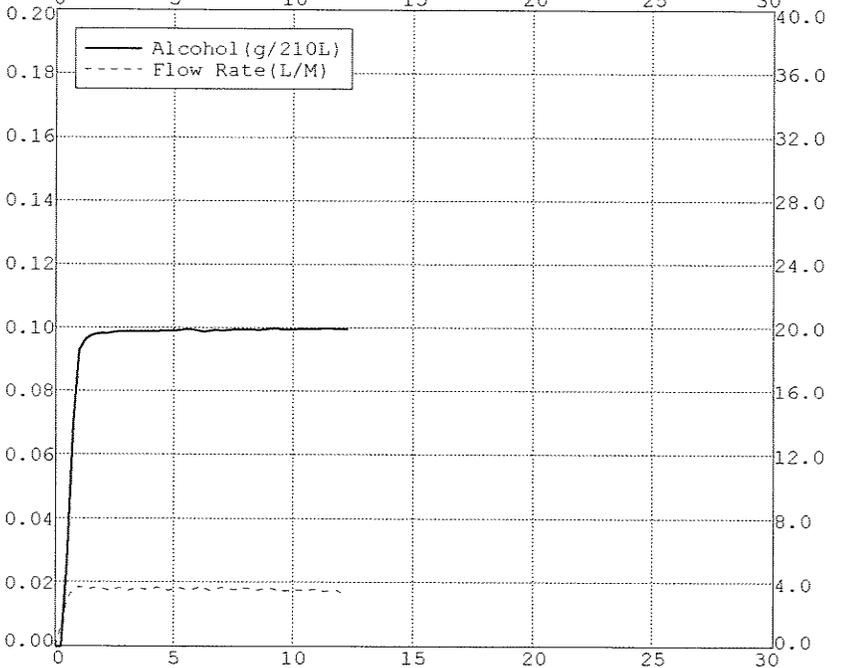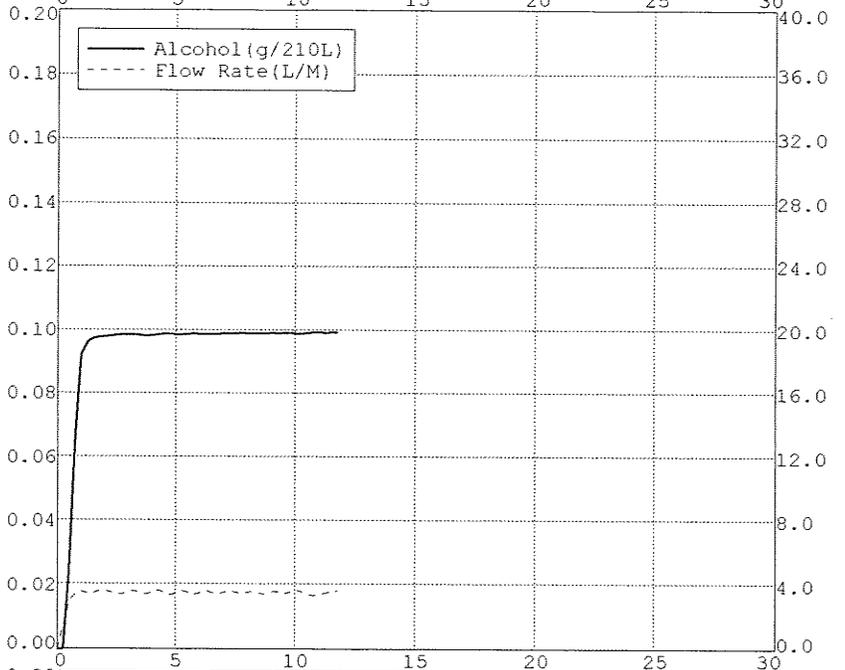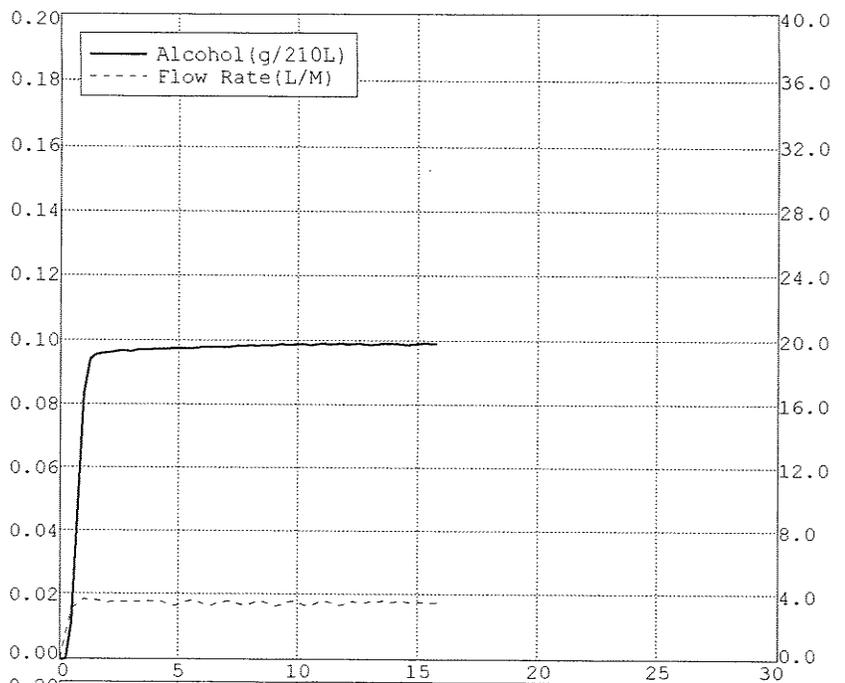

Charles B Geisler #244