

SOLUTION CHANGE



WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 12/05/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 22:44 |
| INTERNAL STANDARD | VERIFIED | 22:44 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 22:45 |
| BLANK TEST | 0.00 | 22:45 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 22:46 |
| BLANK TEST | 0.00 | 22:47 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 22:47 |
| BLANK TEST | 0.00 | 22:48 |

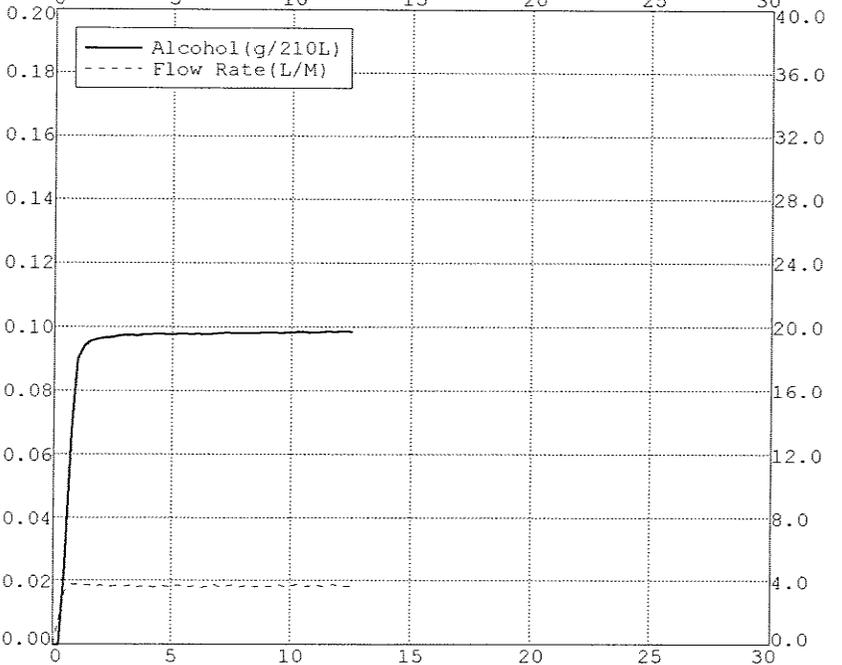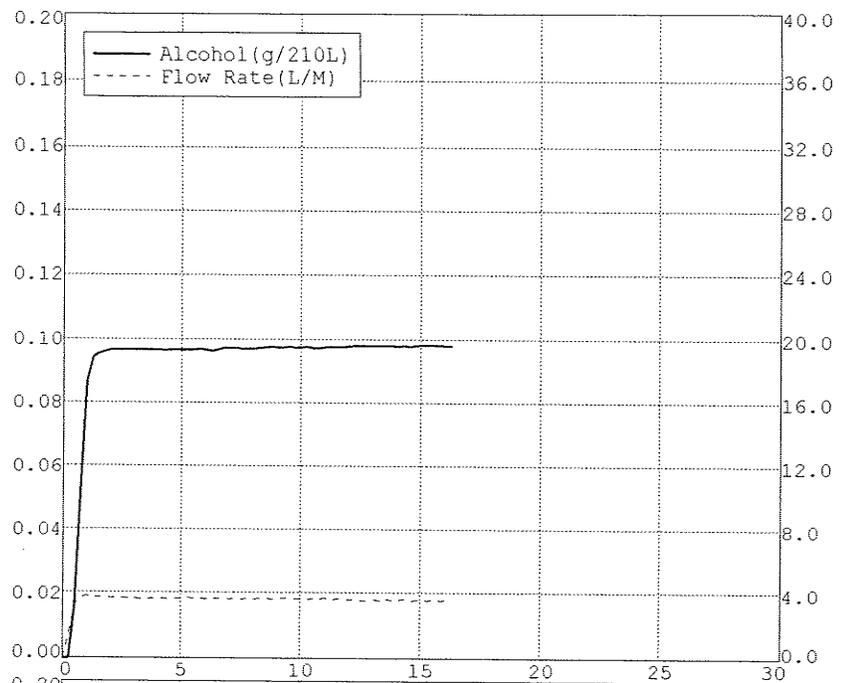

Charles B. Geisler #244