

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 12/11/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:16
INTERNAL STANDARD	VERIFIED	01:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:16
BLANK TEST	0.00	01:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:18
BLANK TEST	0.00	01:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:19
BLANK TEST	0.00	01:20

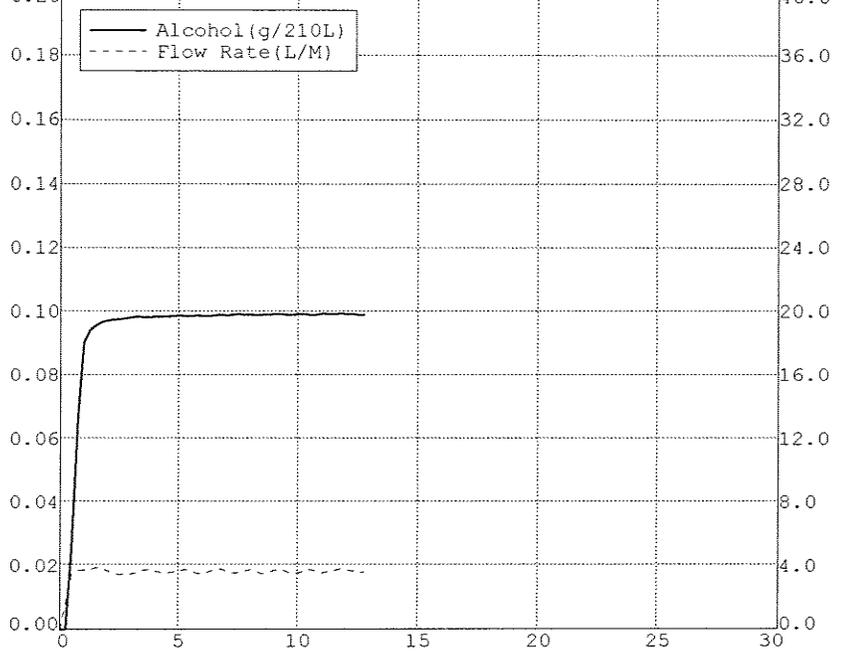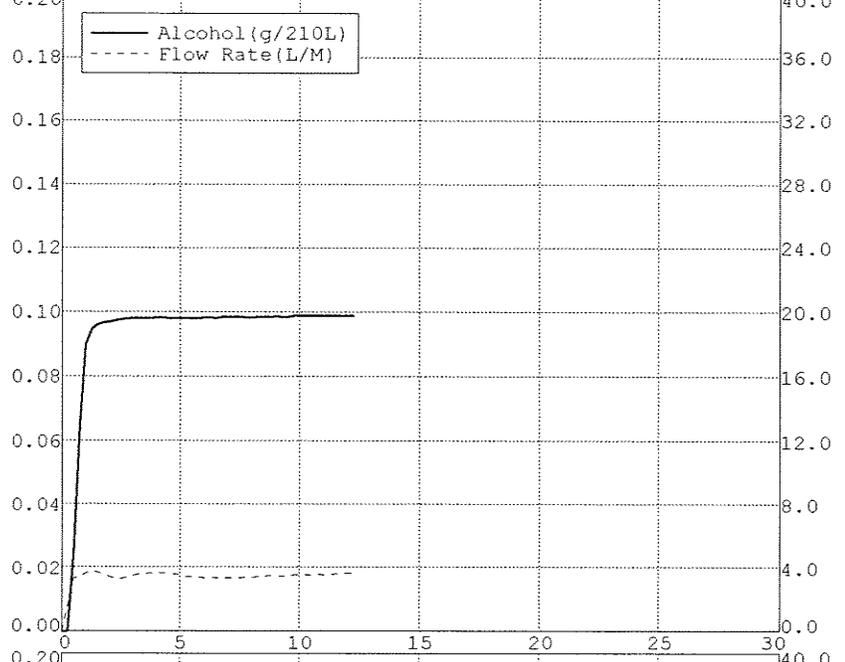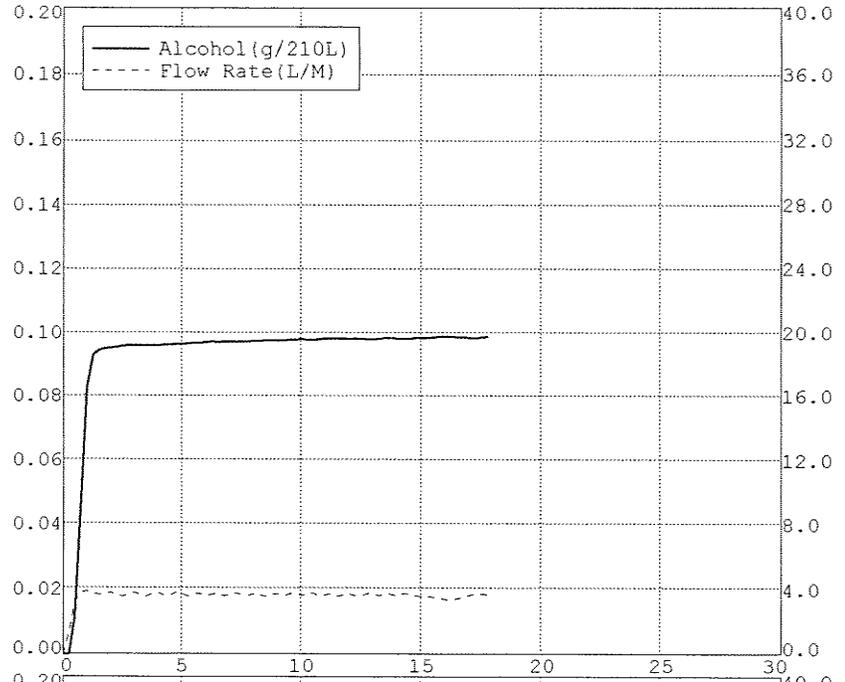

Handwritten signatures and initials:
C. B. Geisler
#20