

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 12/20/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:48
INTERNAL STANDARD	VERIFIED	00:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:48
BLANK TEST	0.00	00:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:50
BLANK TEST	0.00	00:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:51
BLANK TEST	0.00	00:52

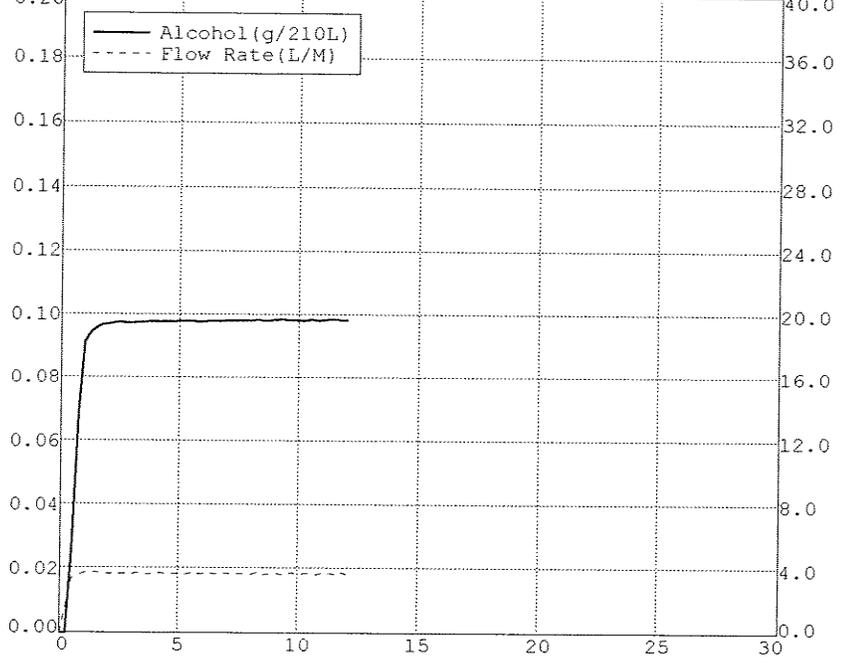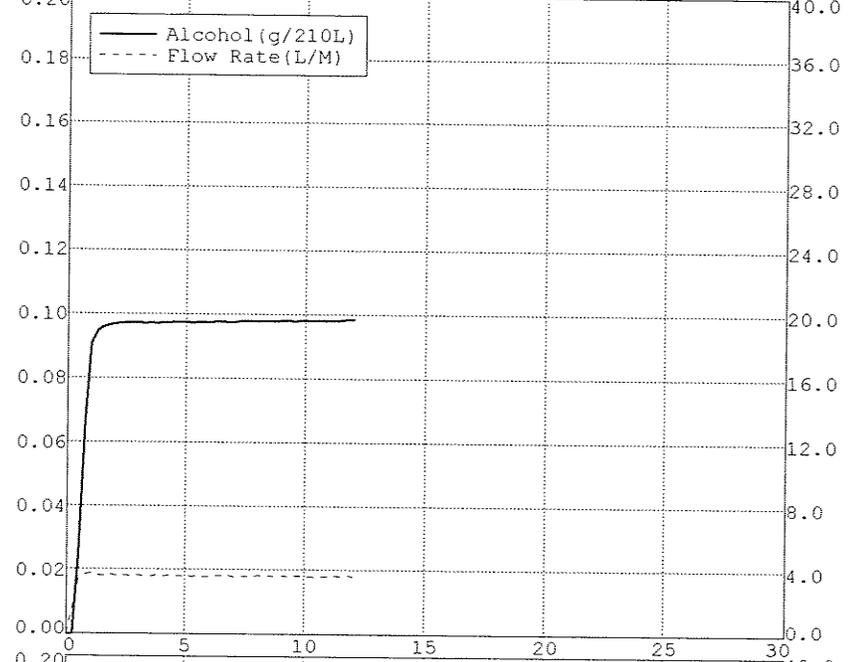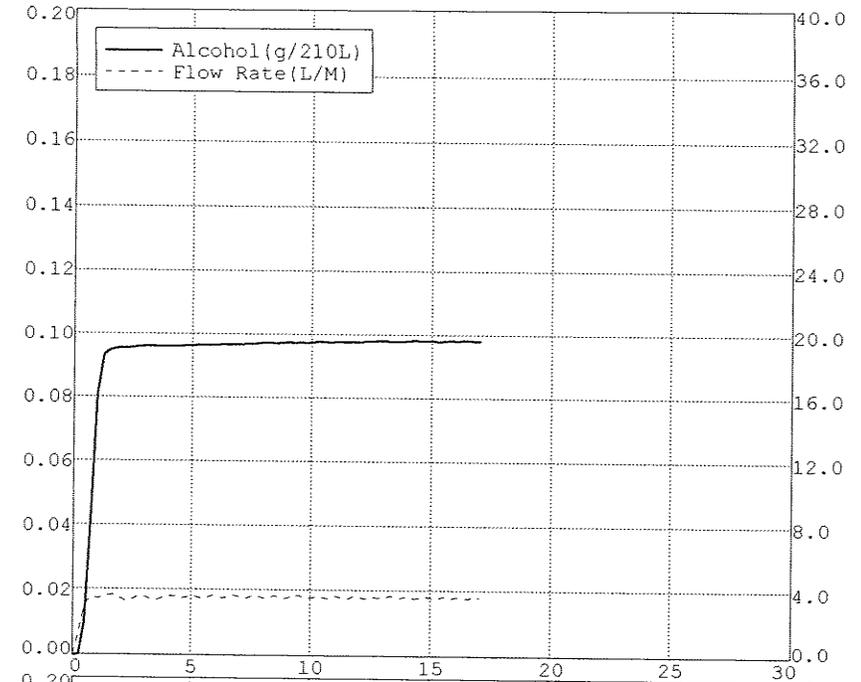

Charles B Geisler *[Signature]*