

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 01/02/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:34
INTERNAL STANDARD	VERIFIED	21:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:34
BLANK TEST	0.00	21:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:36
BLANK TEST	0.00	21:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:37
BLANK TEST	0.00	21:38

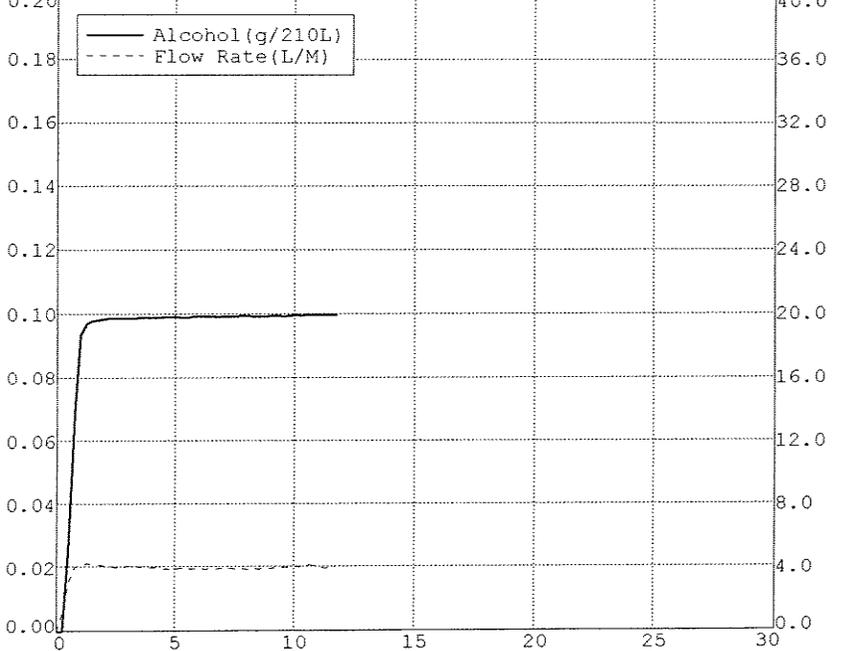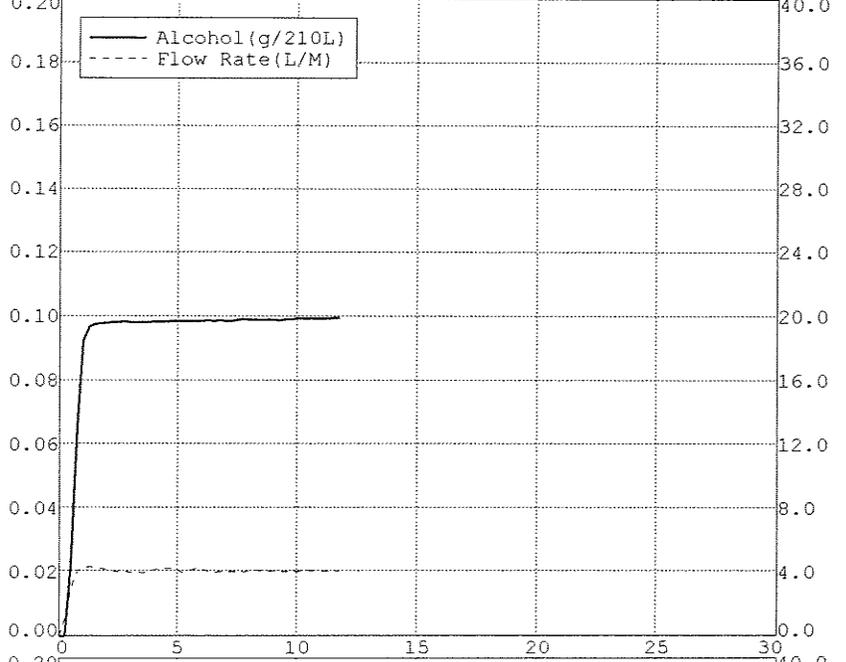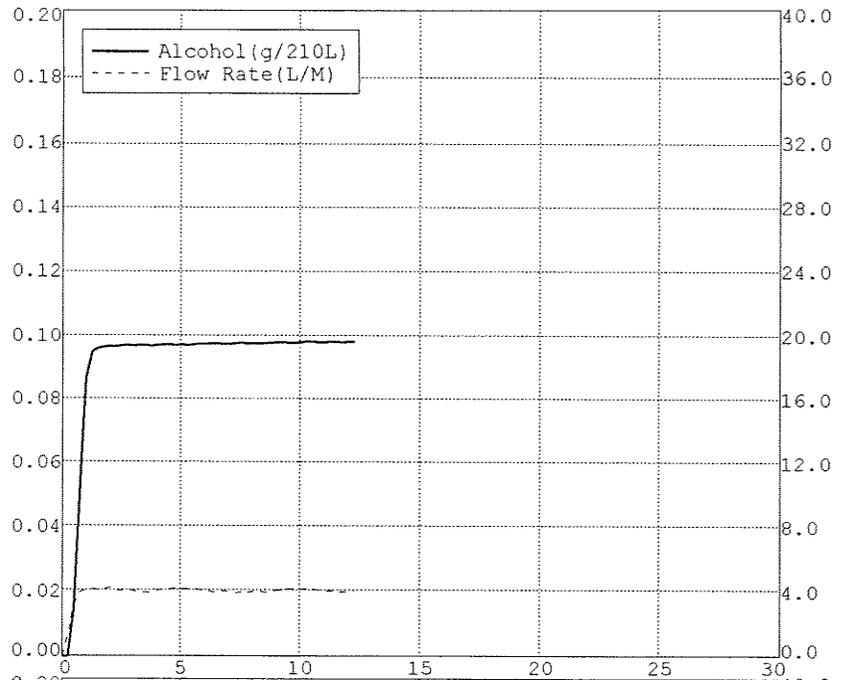

*Charles B. Geisler*