

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 01/07/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:36
INTERNAL STANDARD	VERIFIED	21:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:36
BLANK TEST	0.00	21:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:38
BLANK TEST	0.00	21:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:39
BLANK TEST	0.00	21:40

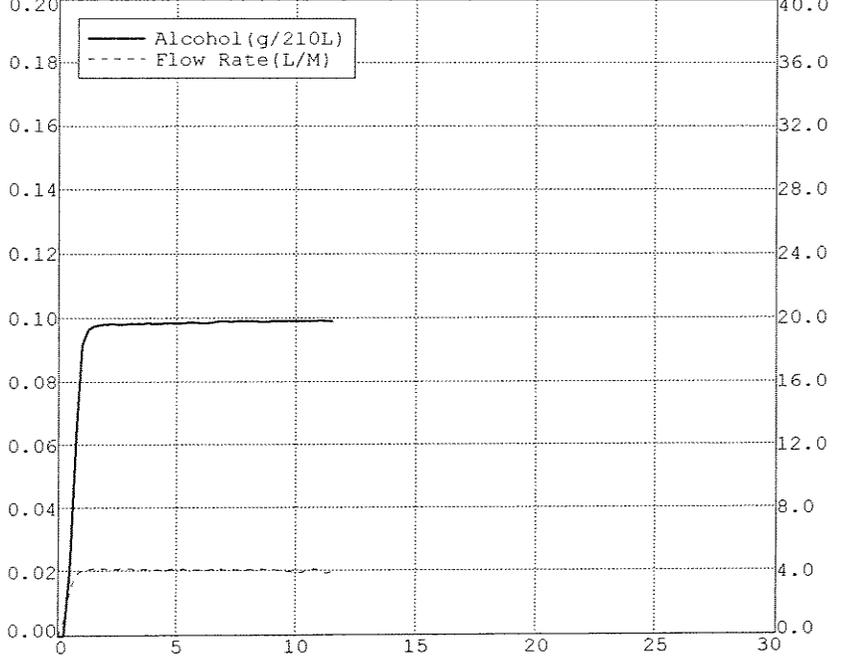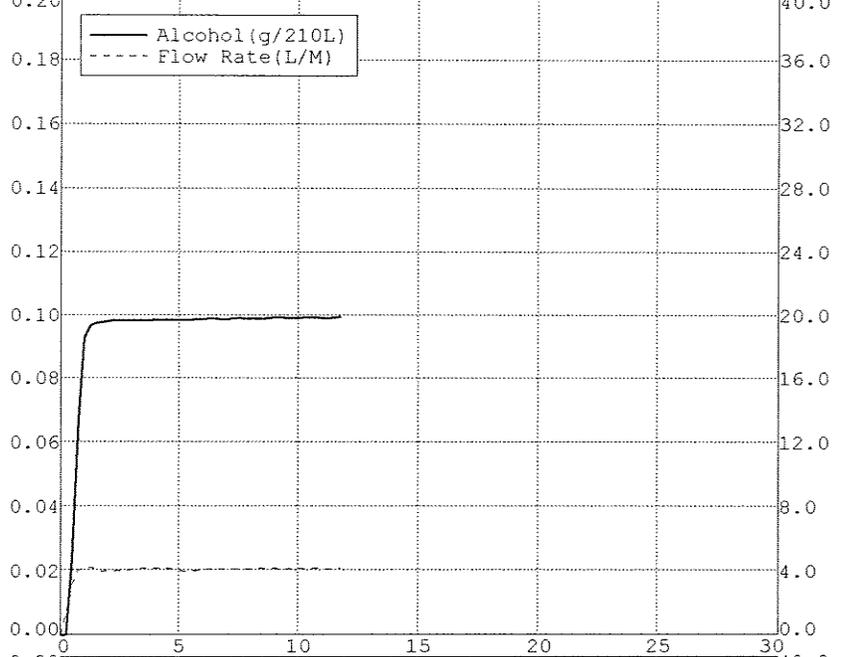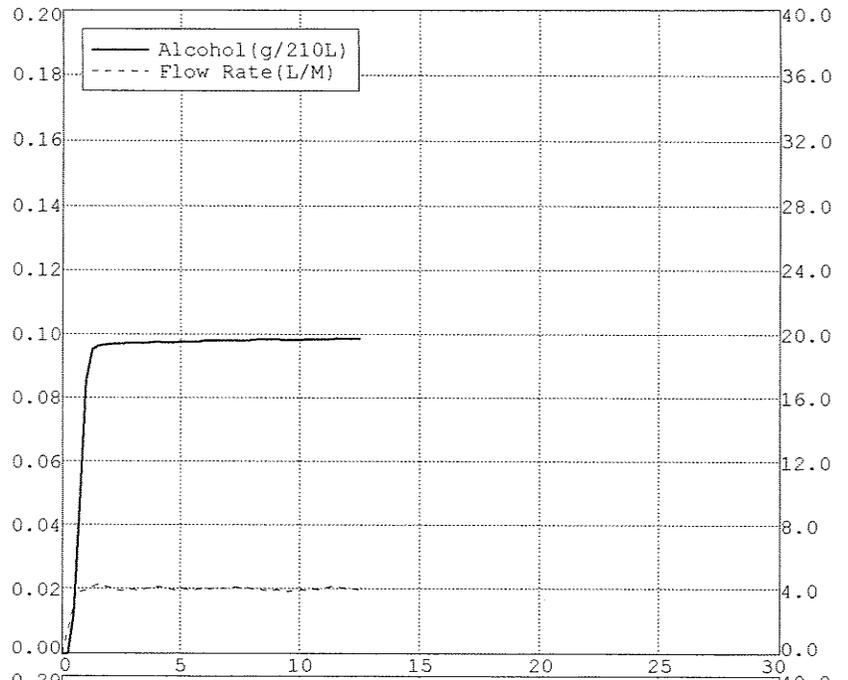

Charles B. Geisler