

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 01/27/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:24
INTERNAL STANDARD	VERIFIED	22:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:25
BLANK TEST	0.00	22:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:26
BLANK TEST	0.00	22:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:28
BLANK TEST	0.00	22:29

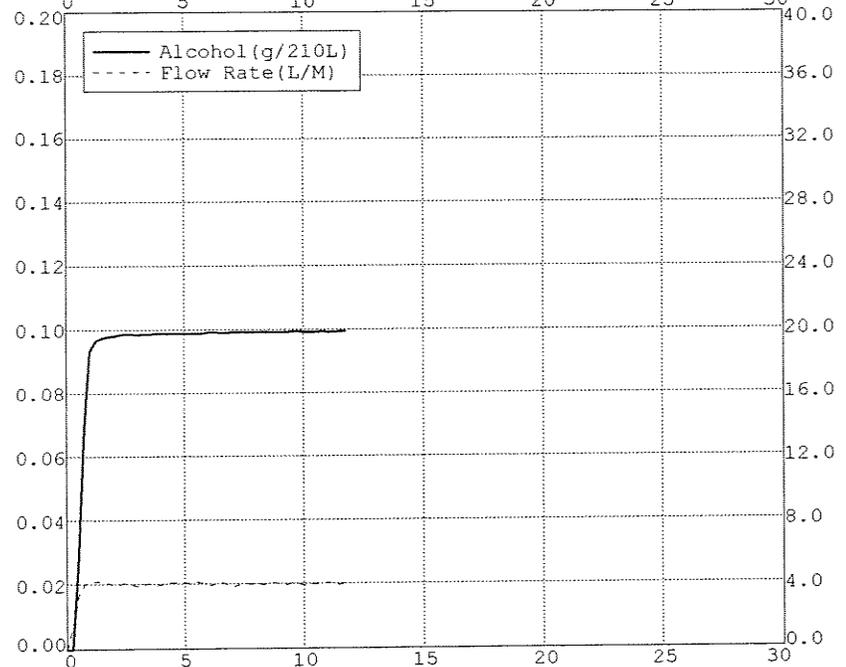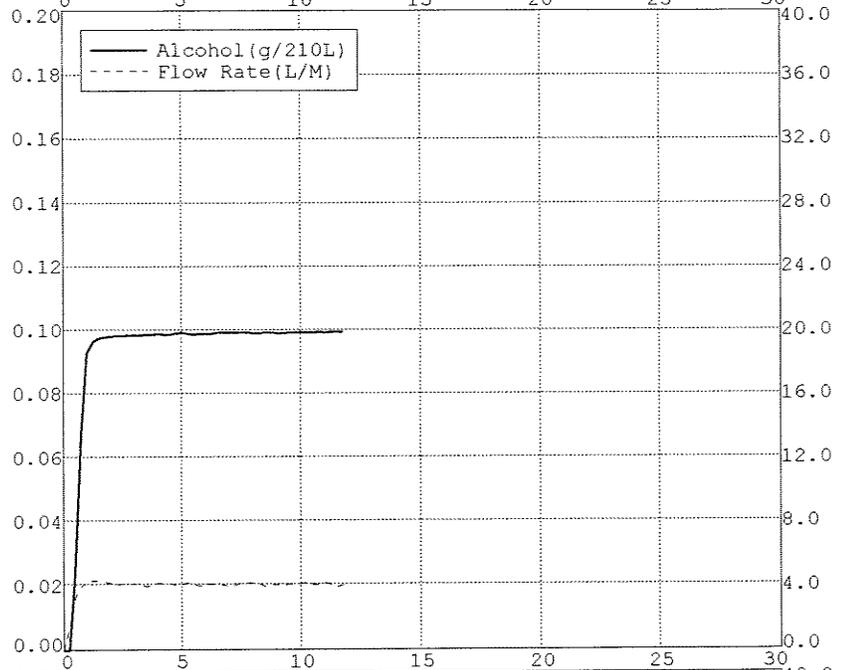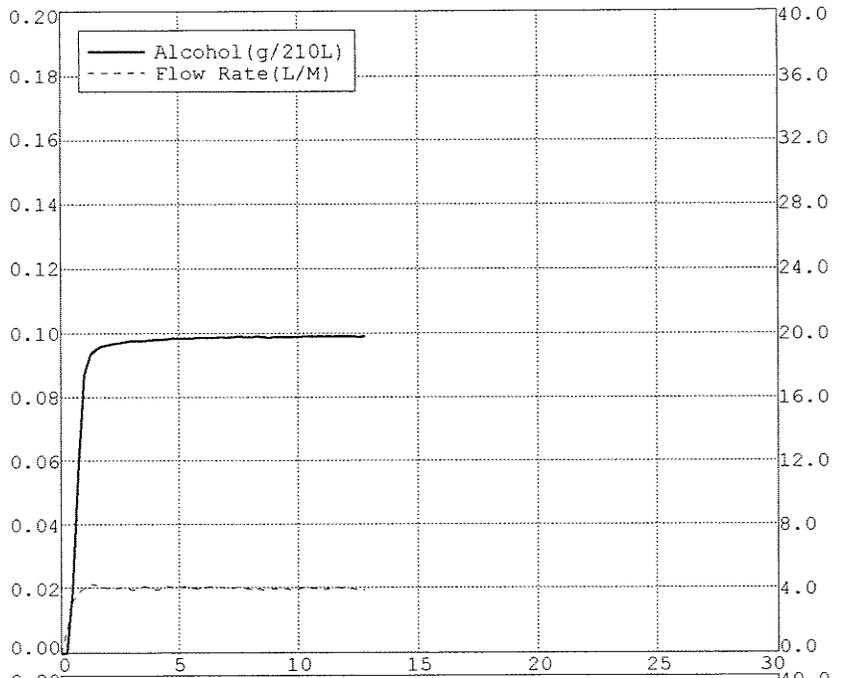

Charles B. Geisler

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 01/27/2019

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:11
INTERNAL STANDARD	VERIFIED	22:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.00	22:12
BLANK TEST	0.00	22:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.00	22:13
BLANK TEST	0.00	22:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.00	22:14
BLANK TEST	0.00	22:15

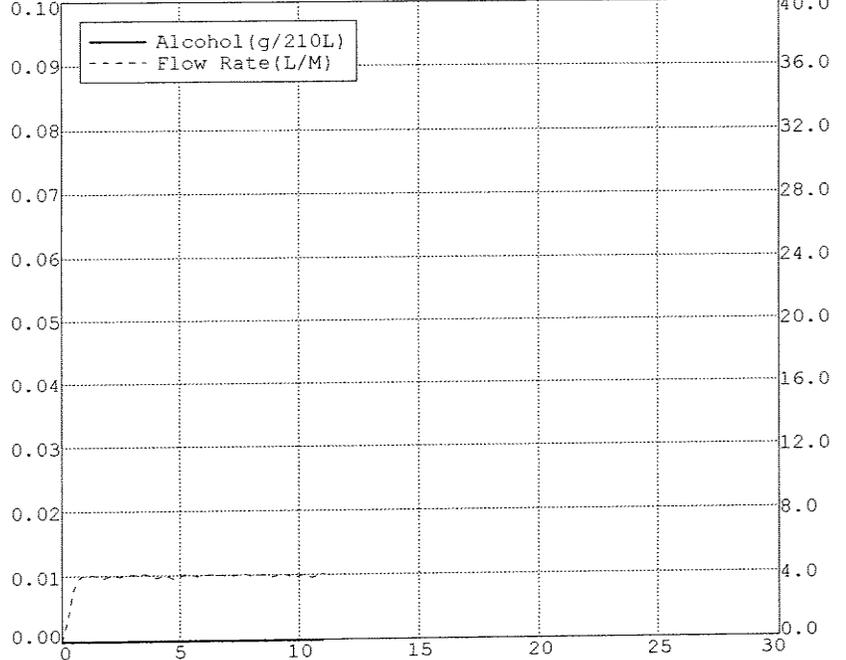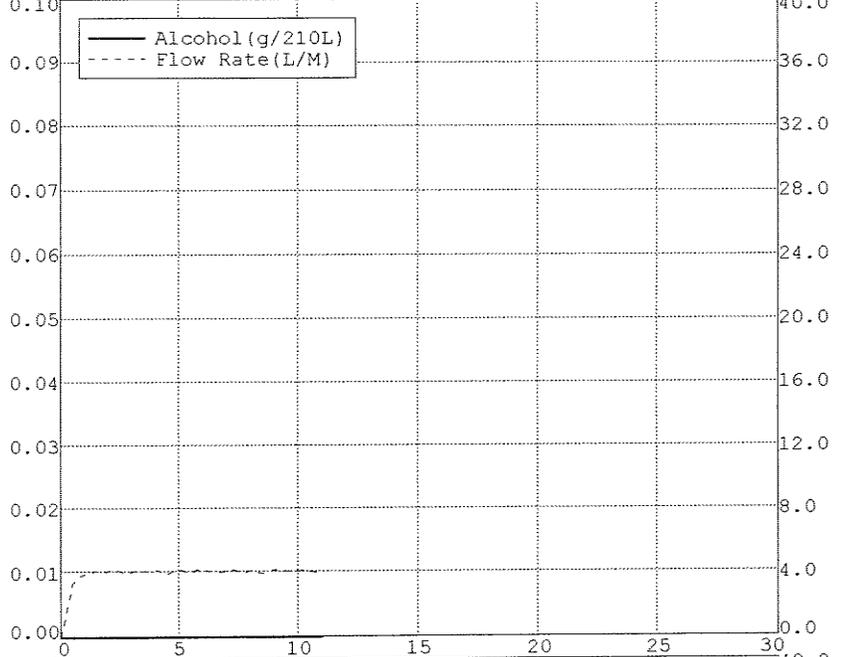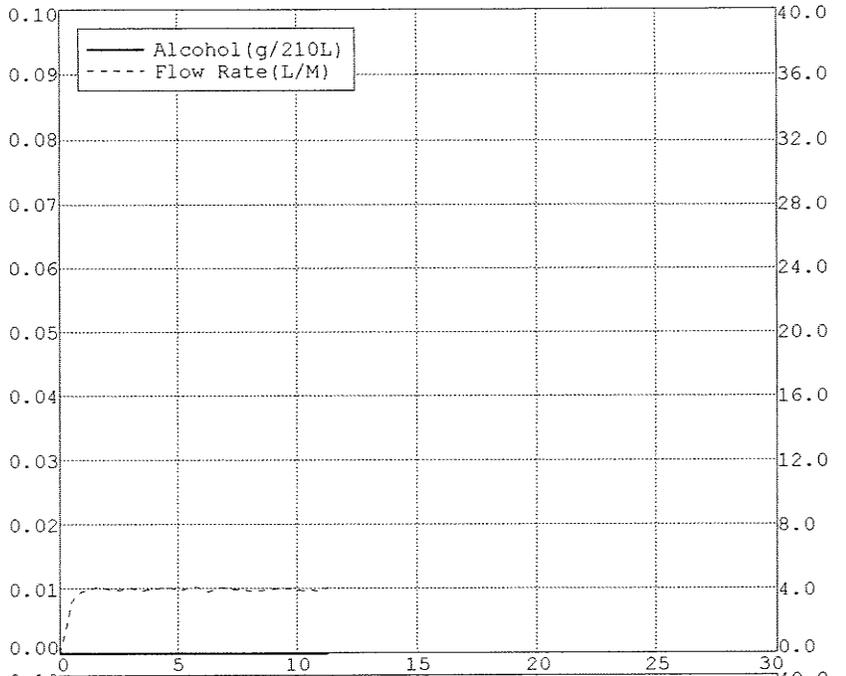

SUPERVISOR TEST

WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 01/27/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:07
INTERNAL STANDARD	VERIFIED	22:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:08

Blank Error

