

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208

Date: 02/10/2019

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:59
INTERNAL STANDARD	VERIFIED	22:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:59
BLANK TEST	0.00	23:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:00
BLANK TEST	0.00	23:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:02
BLANK TEST	0.00	23:03

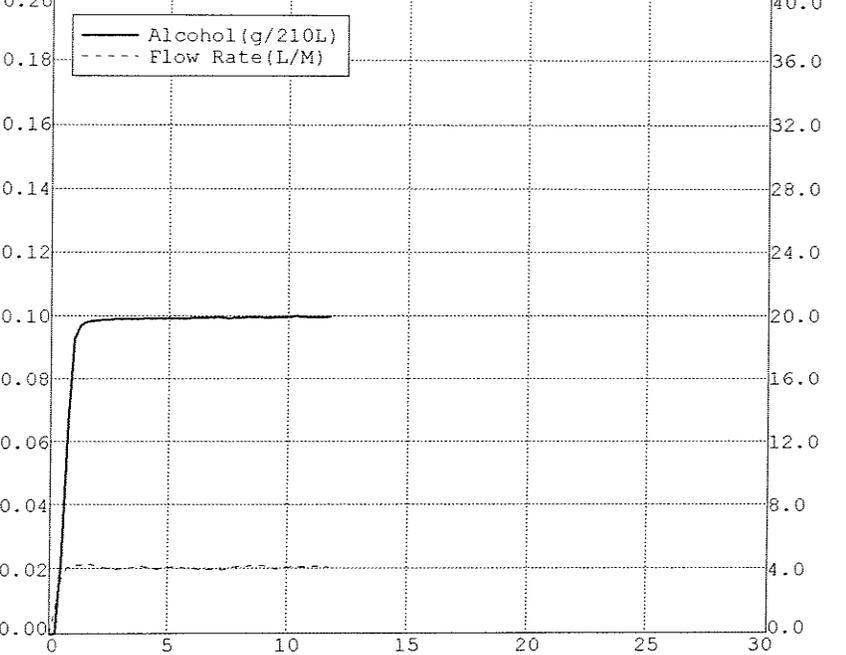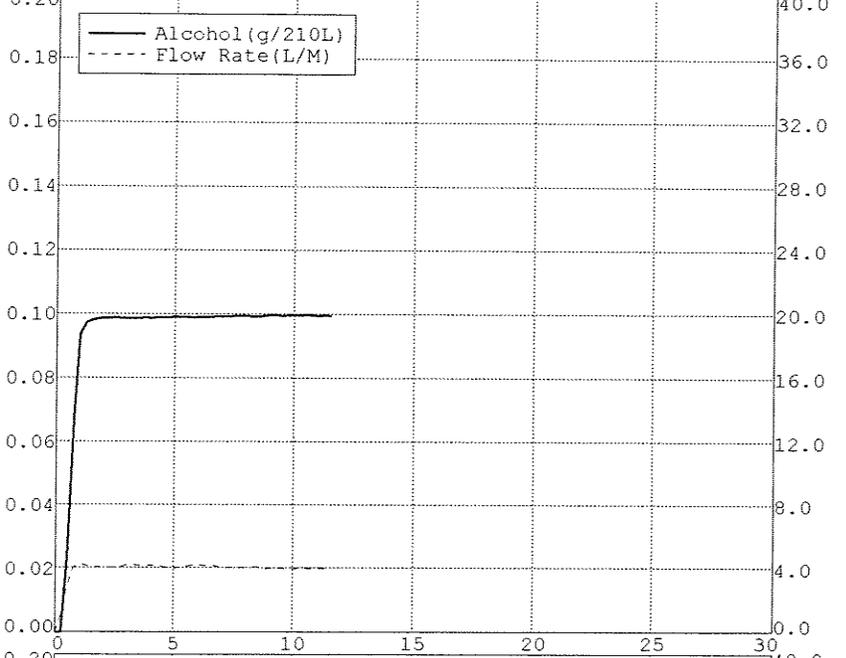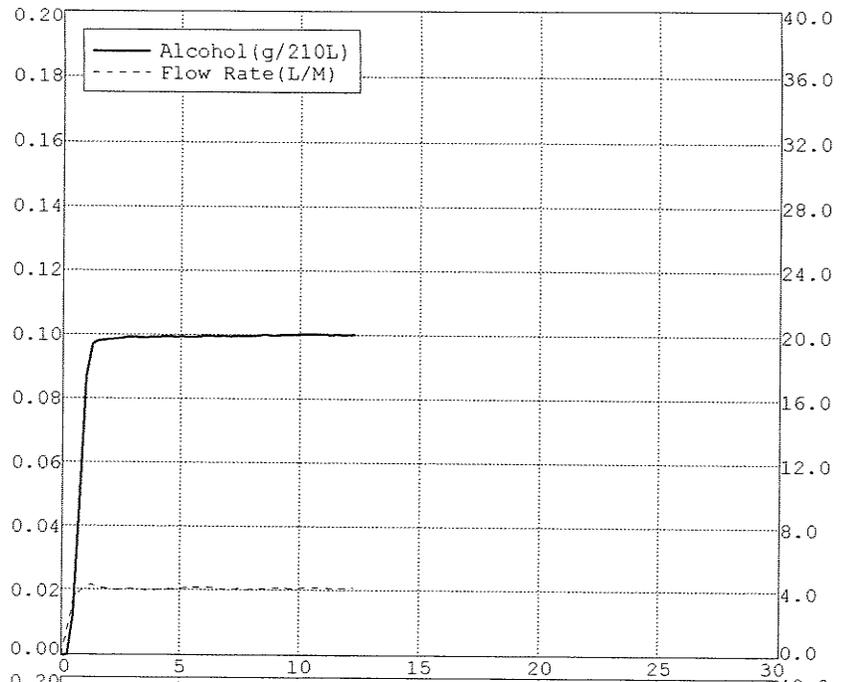

*Handwritten signature: Charles B. Geisler #24*