

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 02/18/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:51
INTERNAL STANDARD	VERIFIED	23:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:51
BLANK TEST	0.00	23:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:53
BLANK TEST	0.00	23:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:54
BLANK TEST	0.00	23:55

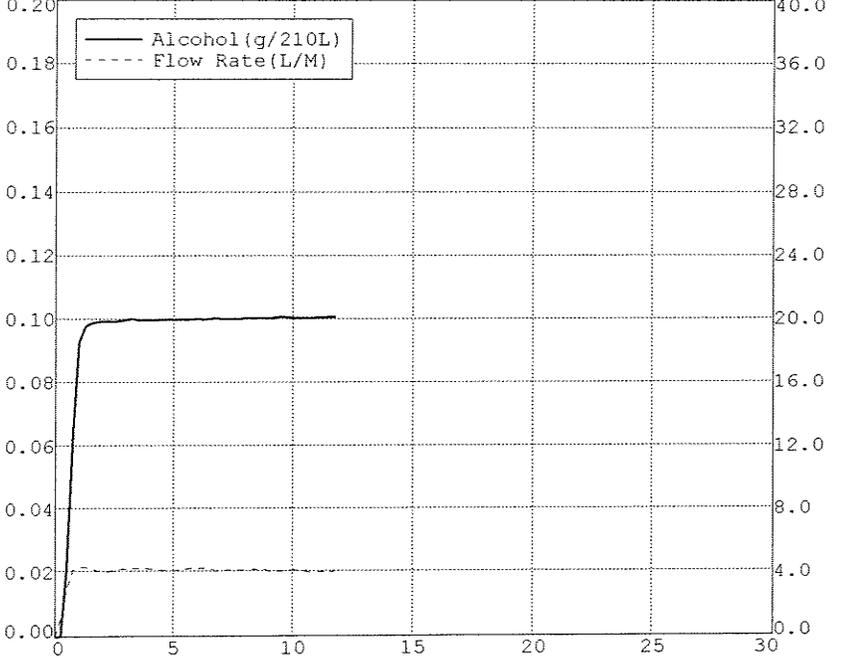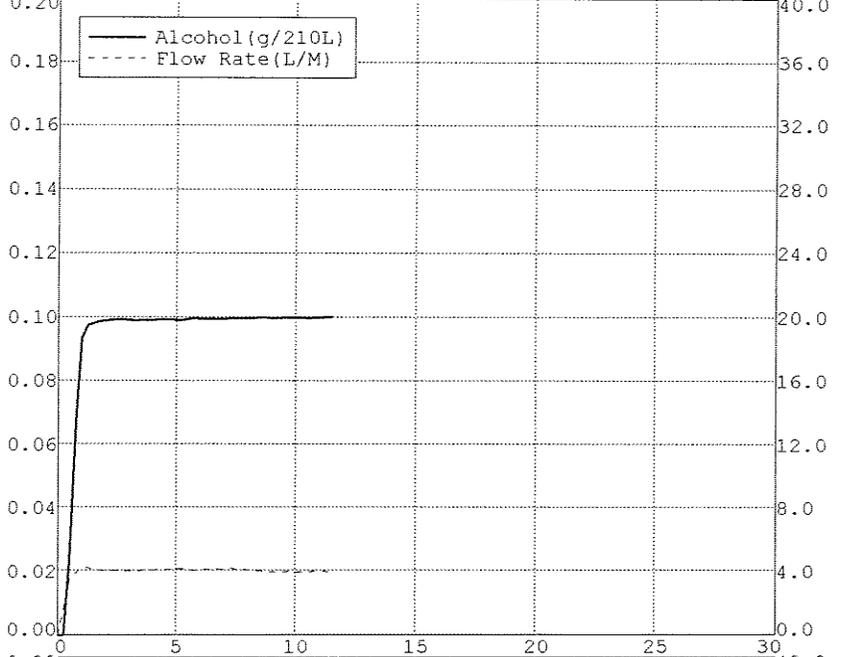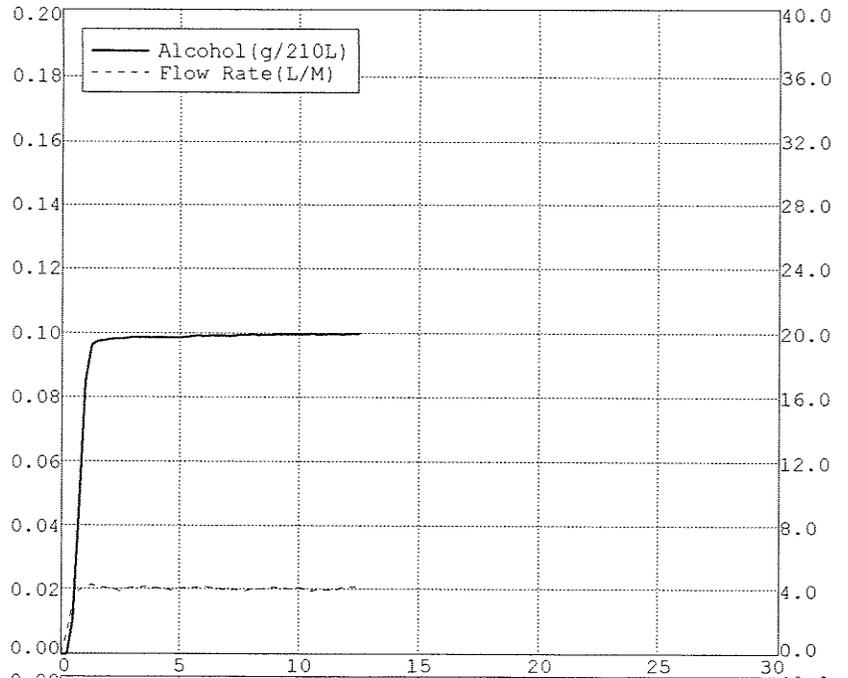

*Signature: Sgt. Charles B. Geisler*