

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 03/15/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:07
INTERNAL STANDARD	VERIFIED	03:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:07
BLANK TEST	0.00	03:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:08
BLANK TEST	0.00	03:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:10
BLANK TEST	0.00	03:11

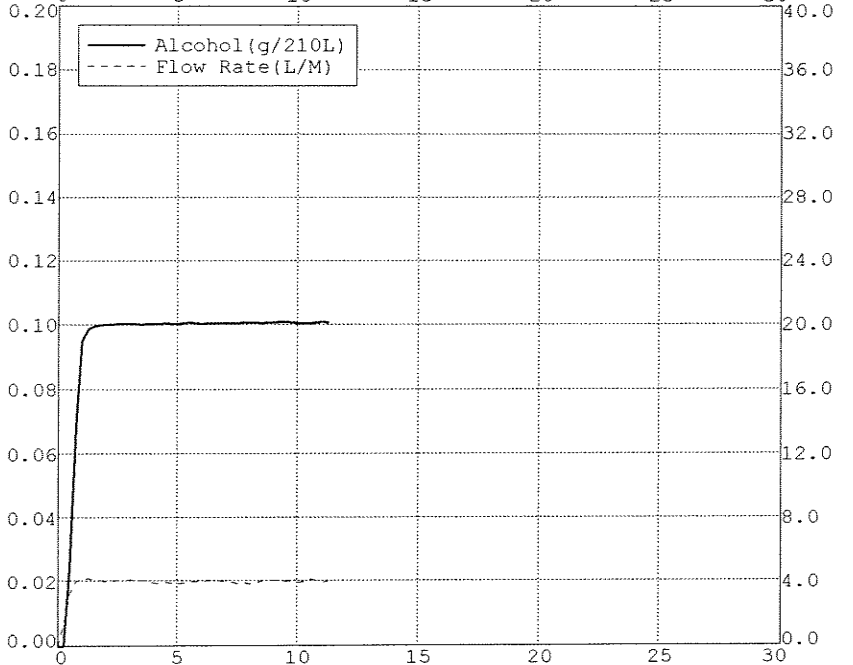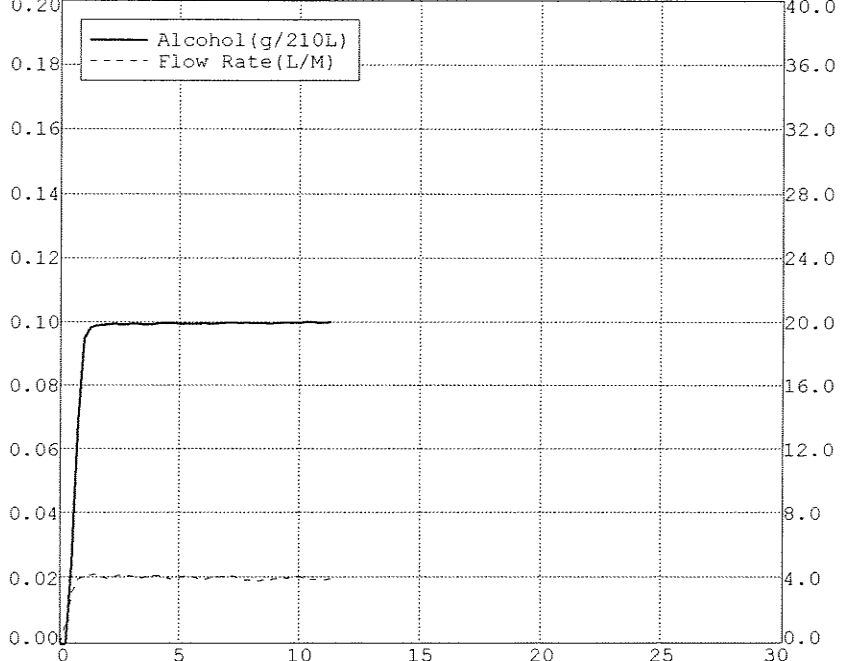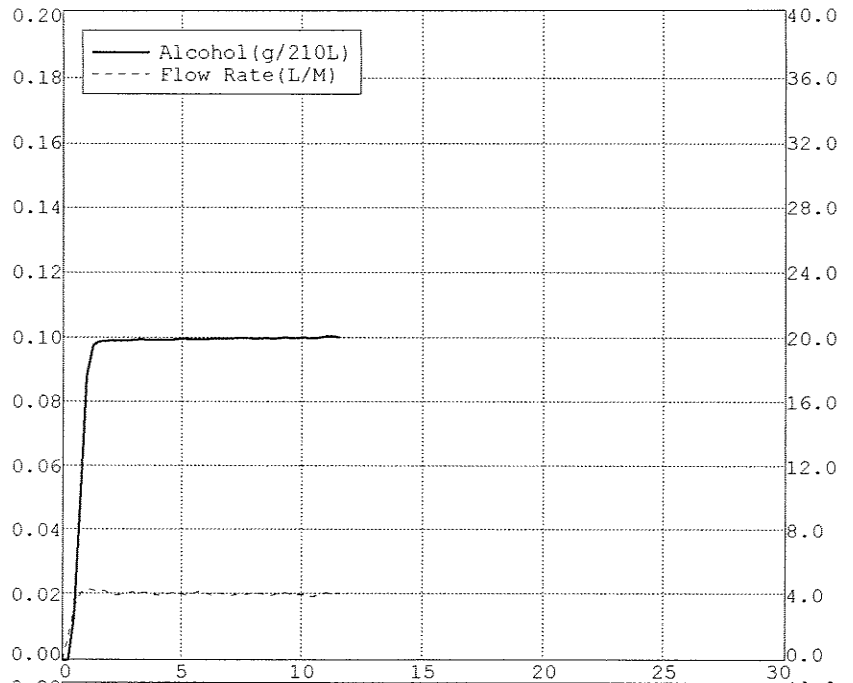

*Charles B Geisler*