

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208

Date: 04/24/2019

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:13
INTERNAL STANDARD	VERIFIED	23:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:14
BLANK TEST	0.00	23:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:15
BLANK TEST	0.00	23:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:16
BLANK TEST	0.00	23:17

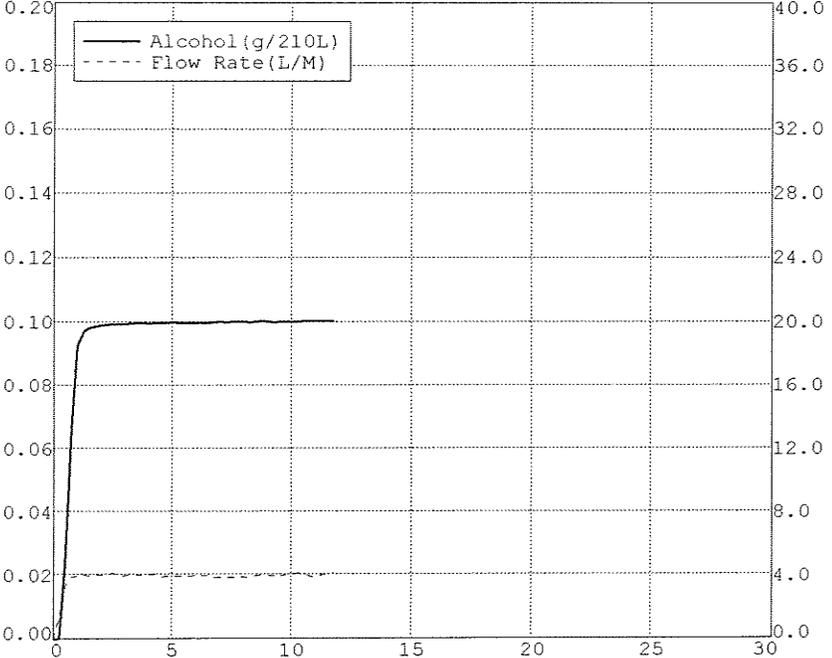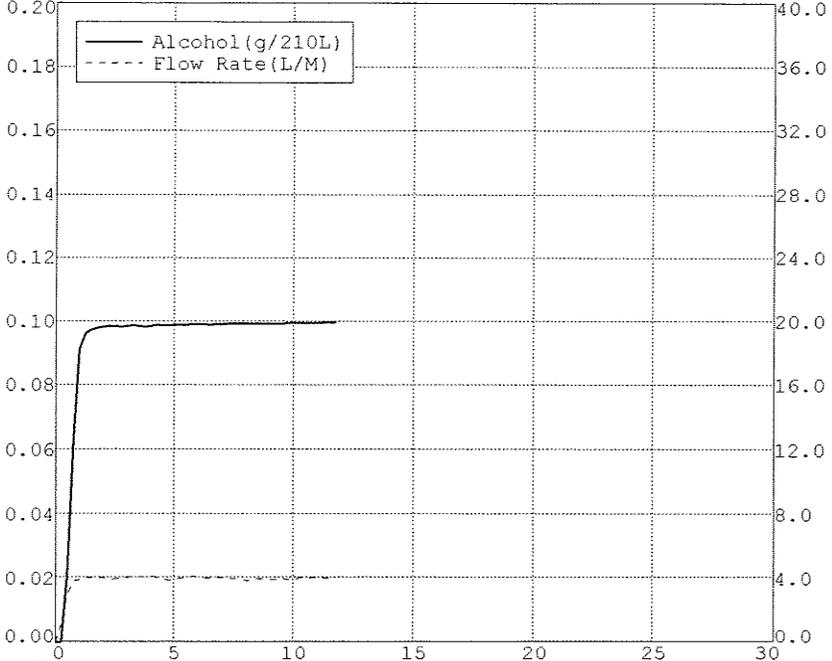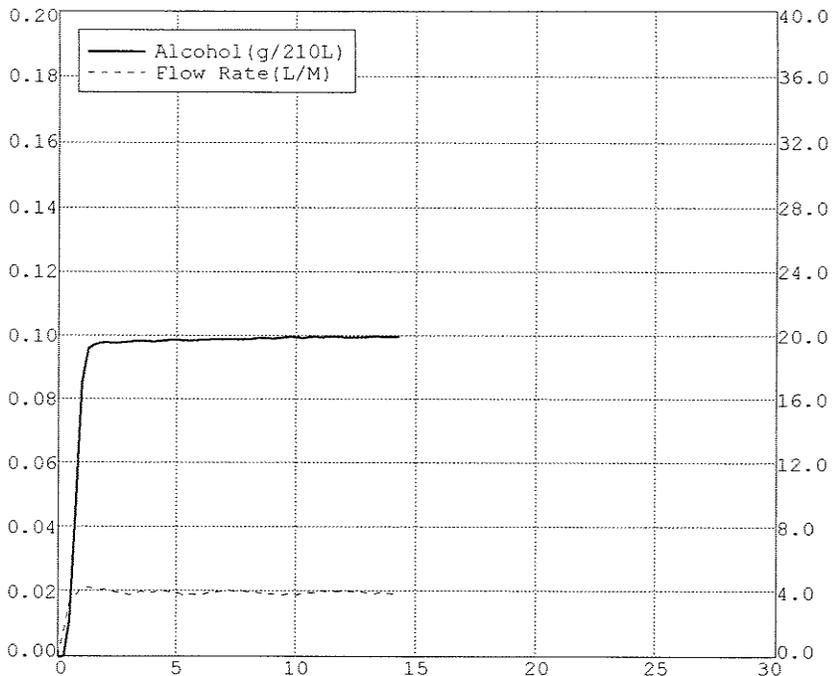

*Charles B. Geisler* #204