

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 05/01/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:48
INTERNAL STANDARD	VERIFIED	03:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:48
BLANK TEST	0.00	03:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:49
BLANK TEST	0.00	03:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:51
BLANK TEST	0.00	03:52

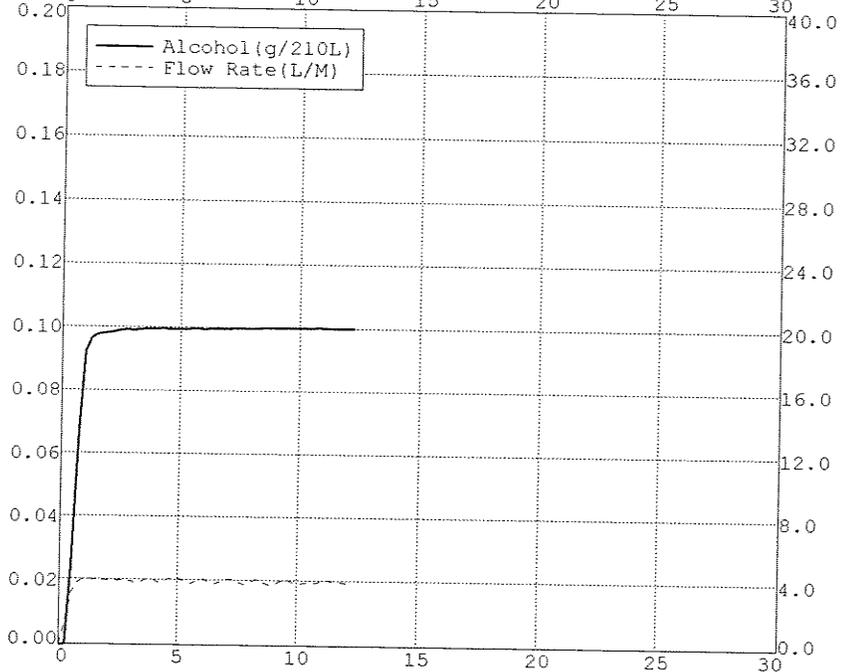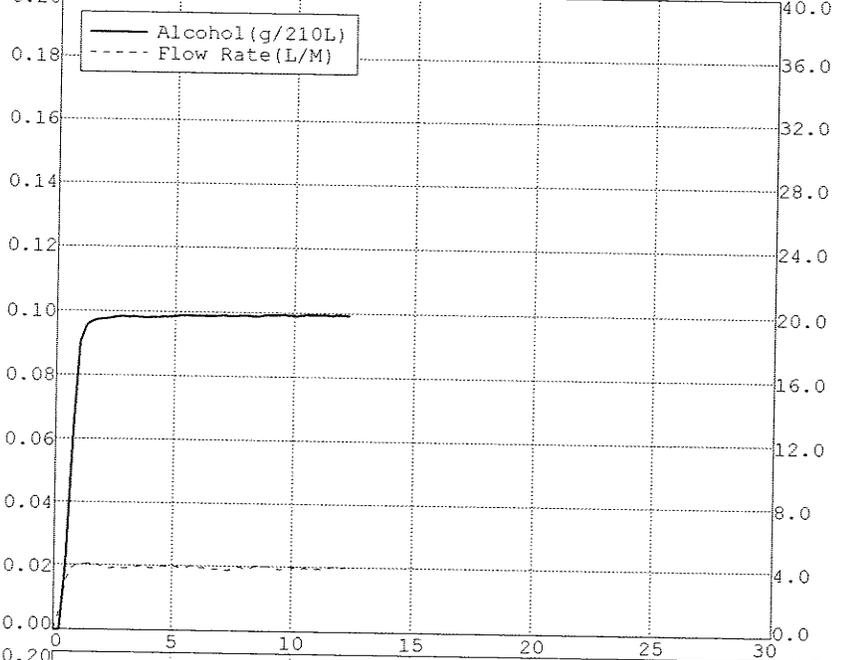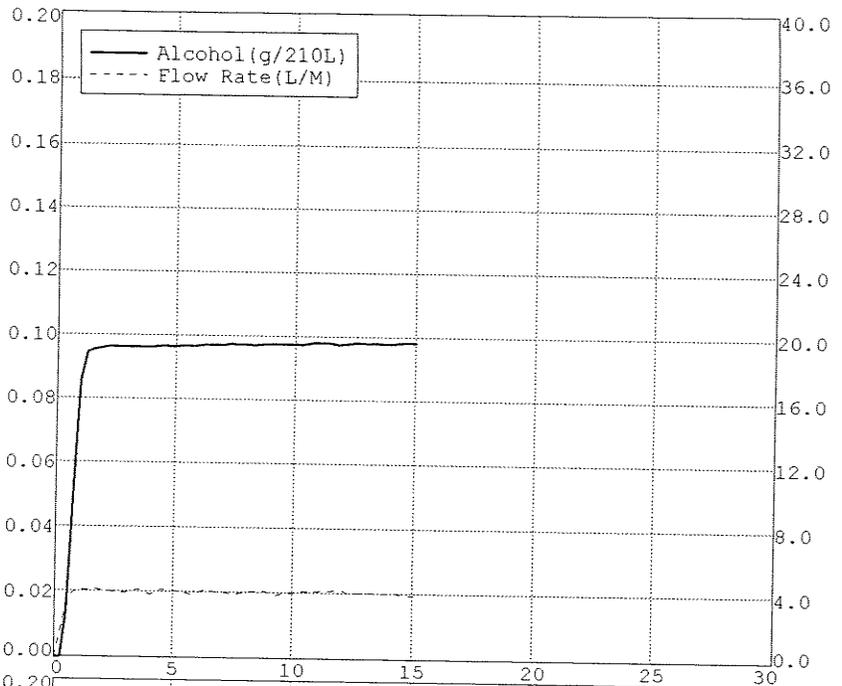

Charles B. Geisler #20