

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 05/08/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:11
INTERNAL STANDARD	VERIFIED	23:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:12
BLANK TEST	0.00	23:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:13
BLANK TEST	0.00	23:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:14
BLANK TEST	0.00	23:15

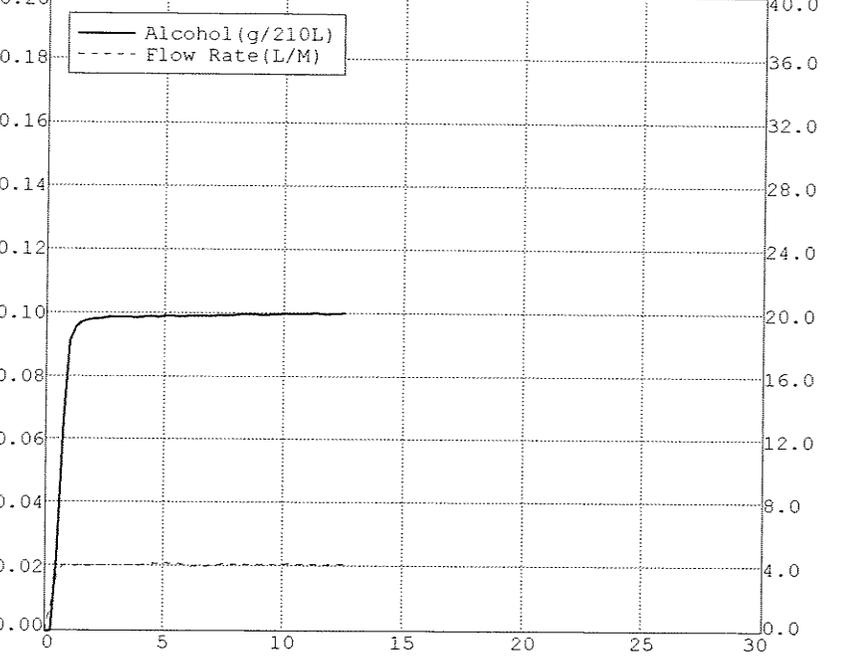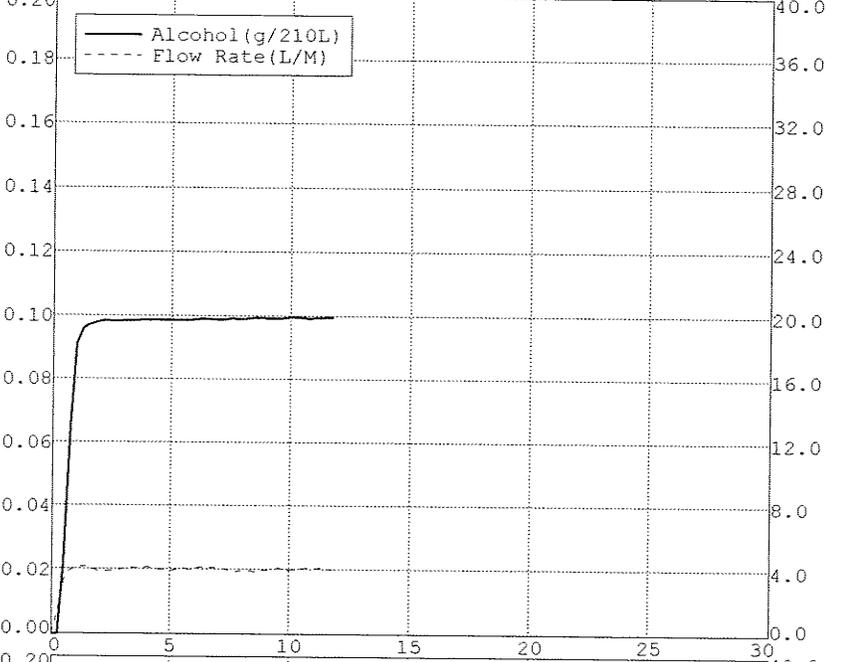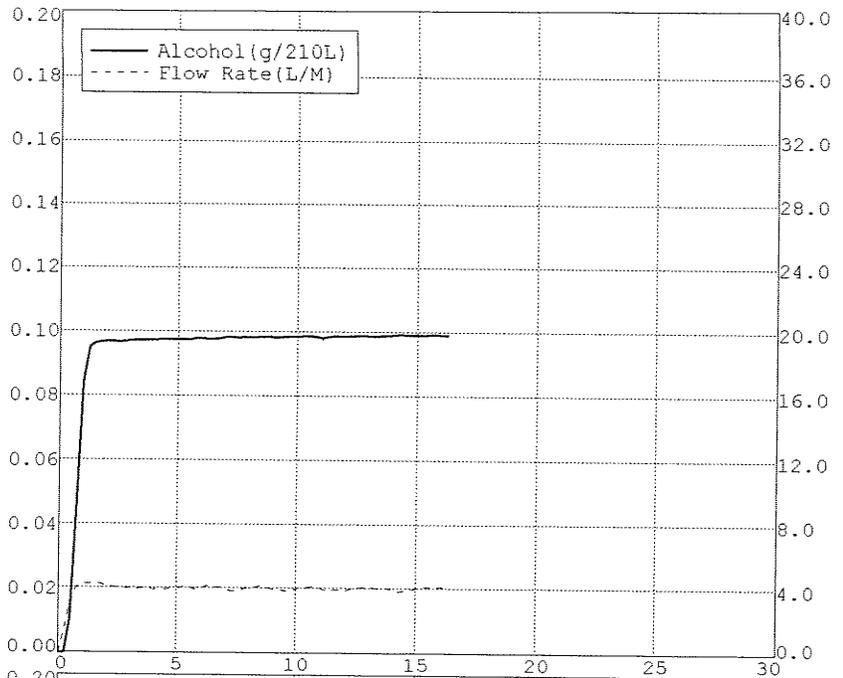

Charles B. Geisler
#241