

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 05/15/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:11
INTERNAL STANDARD	VERIFIED	00:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:11
BLANK TEST	0.00	00:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:13
BLANK TEST	0.00	00:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:14
BLANK TEST	0.00	00:15

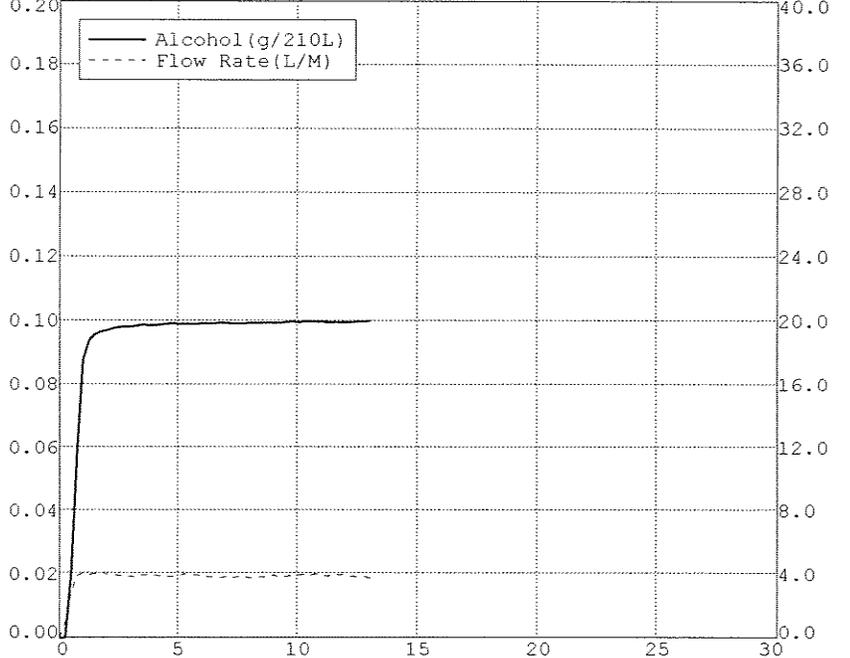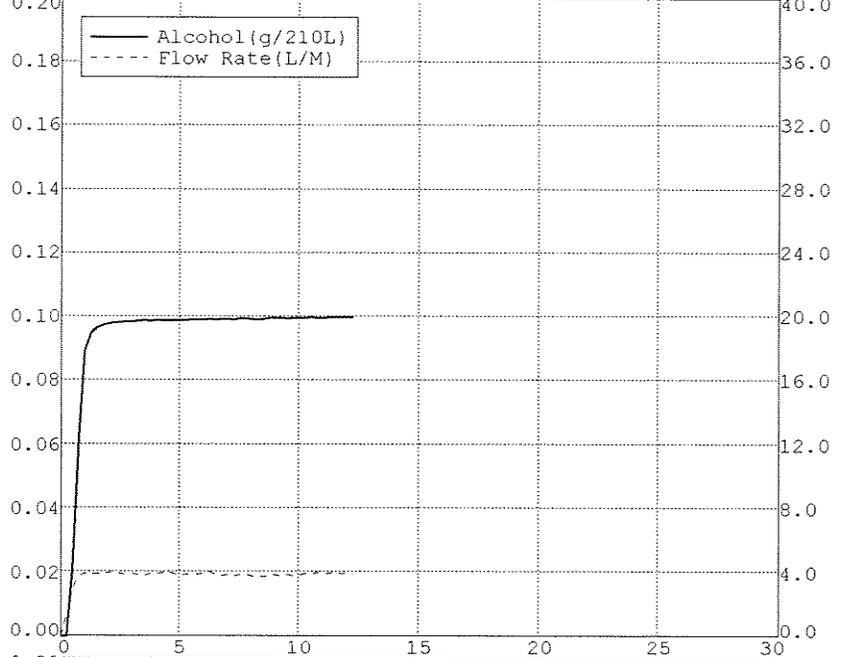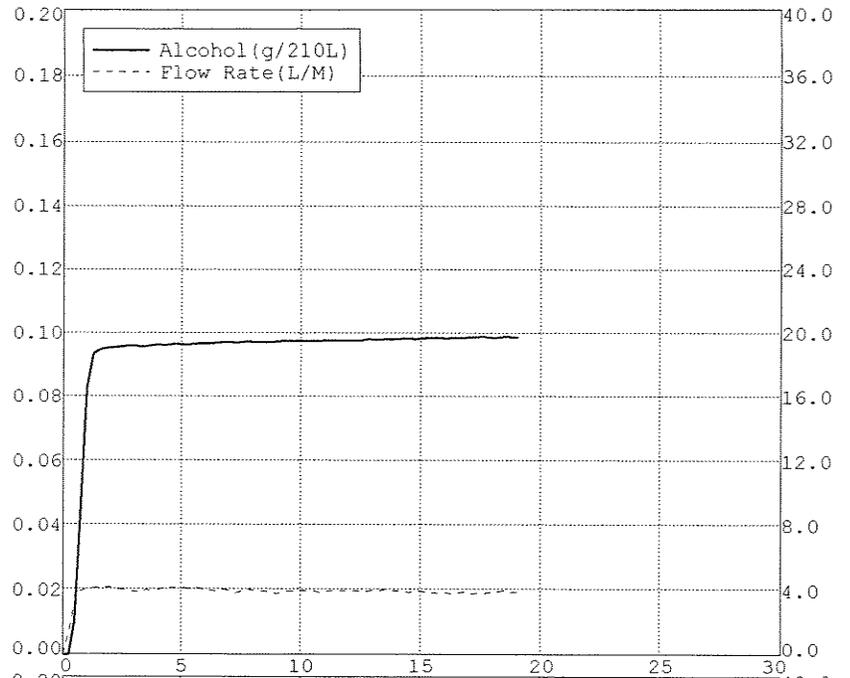

*Charles B. Geisler #20*