

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 05/29/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19030

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:52
INTERNAL STANDARD	VERIFIED	00:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:52
BLANK TEST	0.00	00:53
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	00:54
BLANK TEST	0.00	00:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:55
BLANK TEST	0.00	00:56

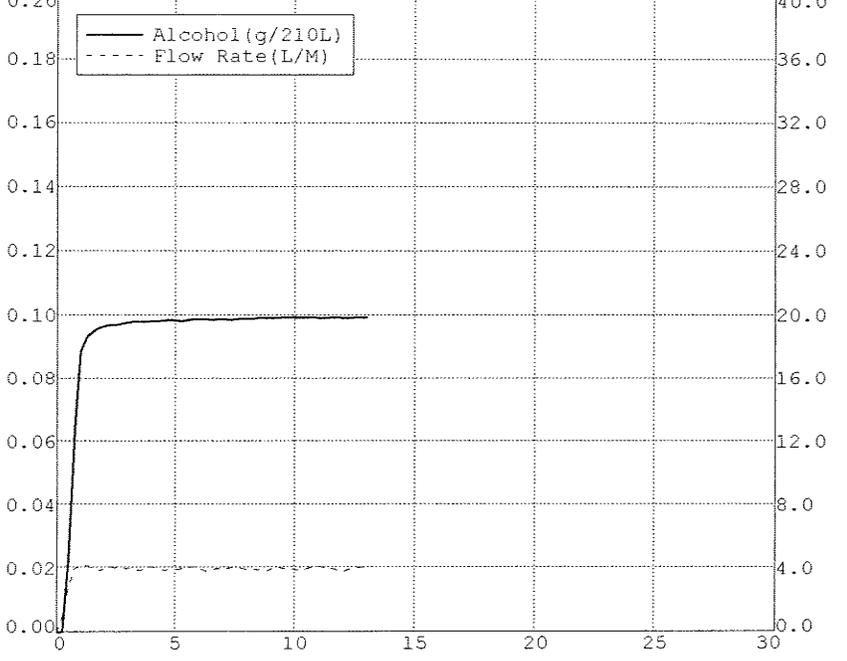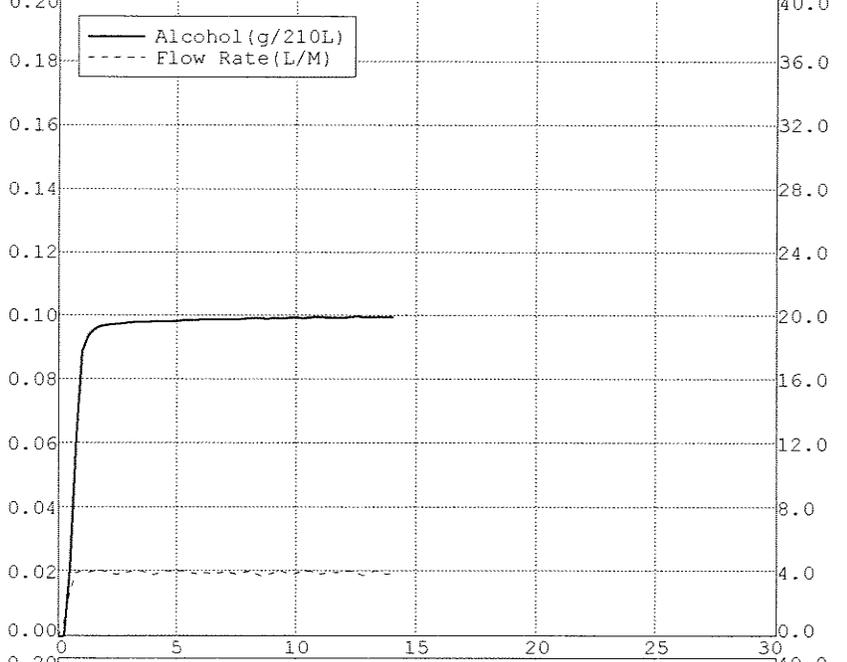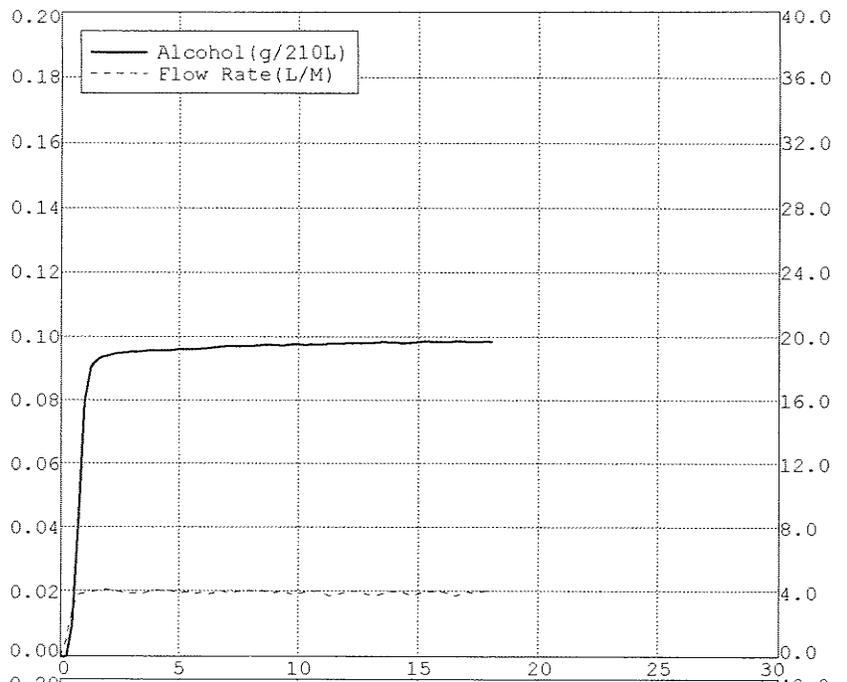

Charles B. Geisler #2W