

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/01/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:15
INTERNAL STANDARD	VERIFIED	23:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:15
BLANK TEST	0.00	23:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:17
BLANK TEST	0.00	23:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:18
BLANK TEST	0.00	23:19

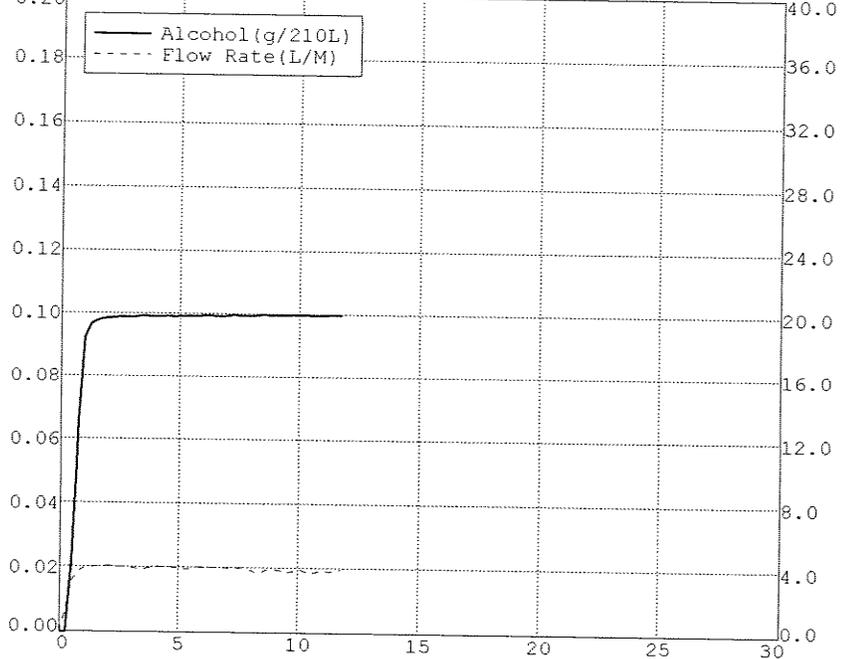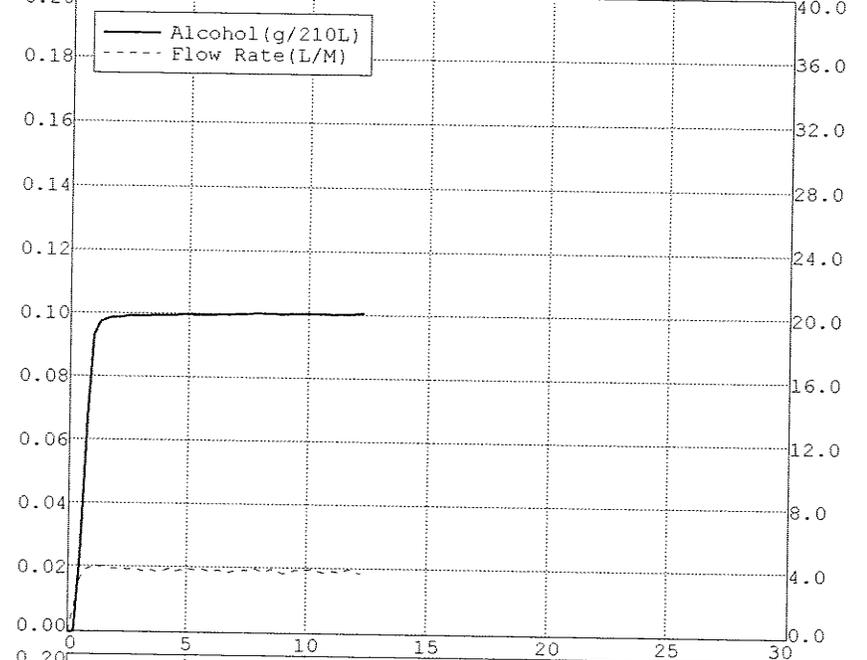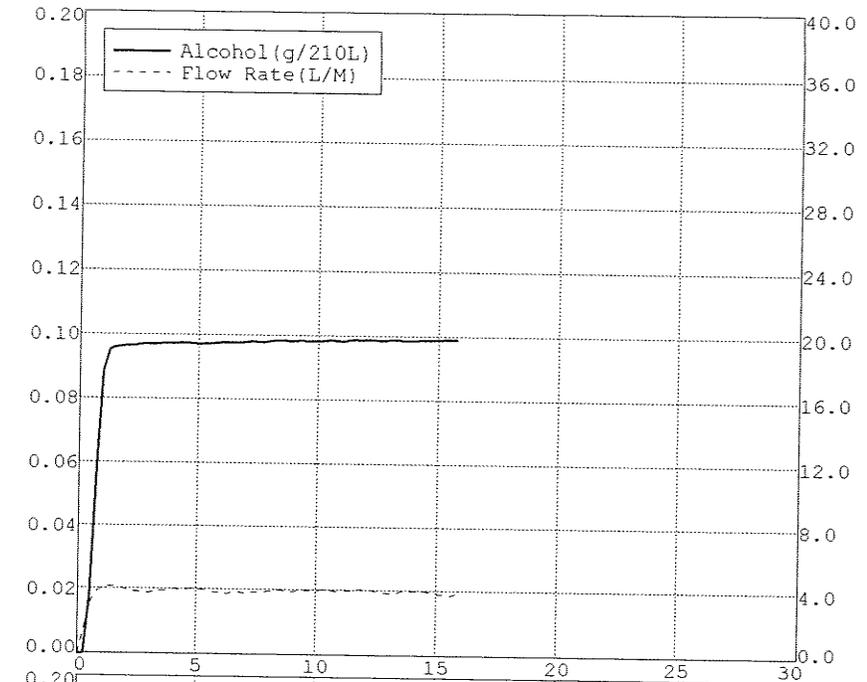

Charles B. Geisler #22W