

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/08/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:53
INTERNAL STANDARD	VERIFIED	16:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:54
BLANK TEST	0.00	16:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:55
BLANK TEST	0.00	16:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:56
BLANK TEST	0.00	16:57

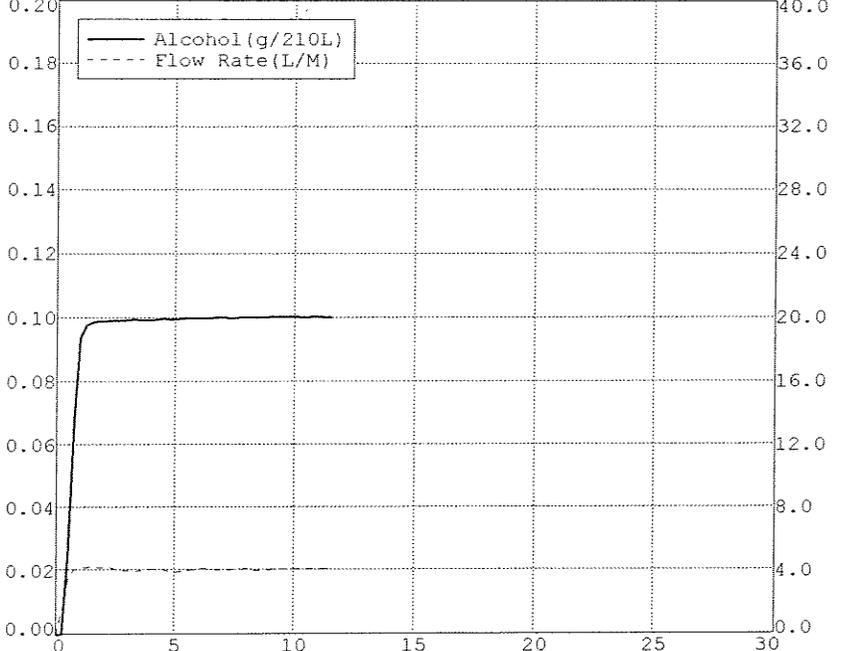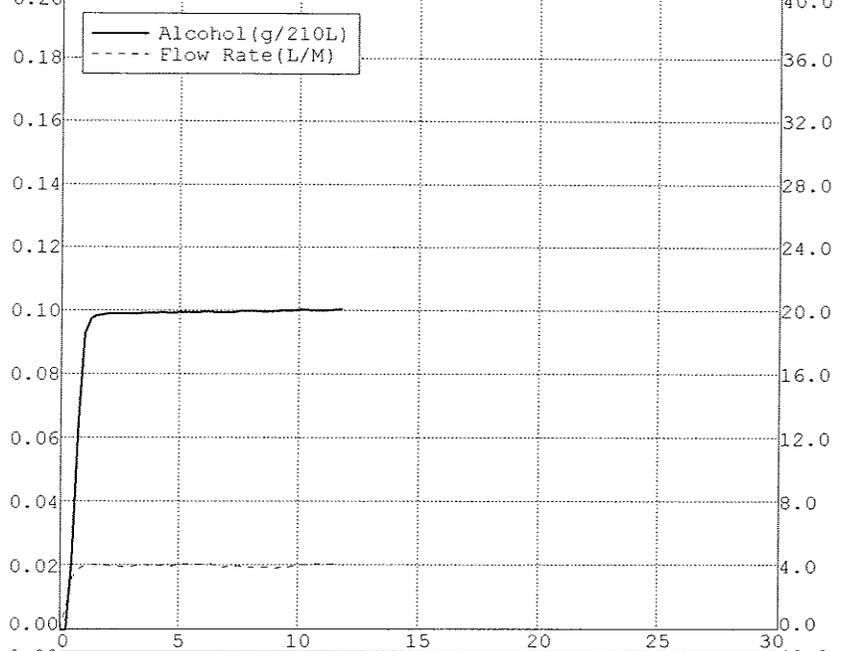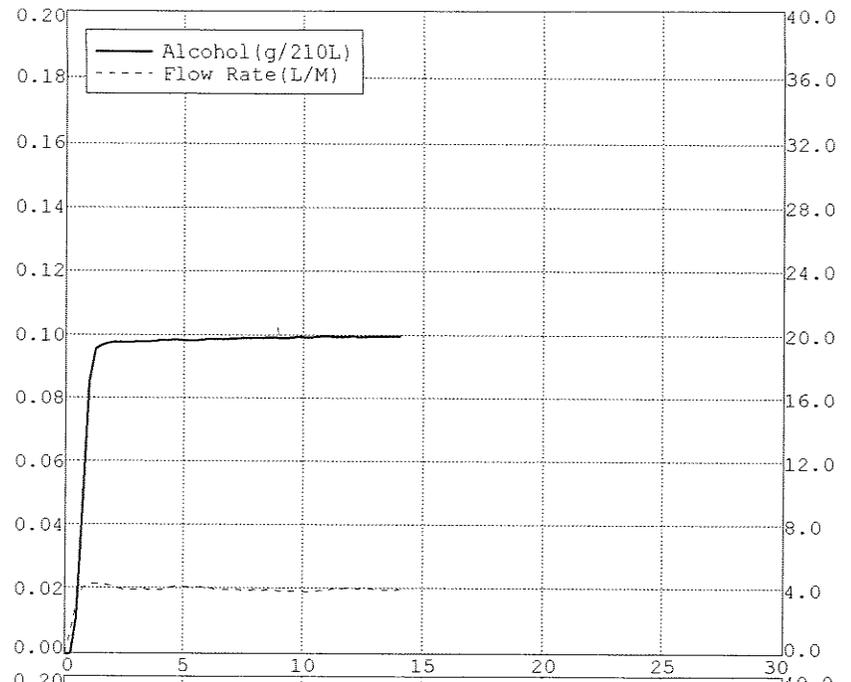

Charles B. Geisler #241