

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/24/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:03
INTERNAL STANDARD	VERIFIED	13:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:04
BLANK TEST	0.00	13:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:05
BLANK TEST	0.00	13:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:06
BLANK TEST	0.00	13:07

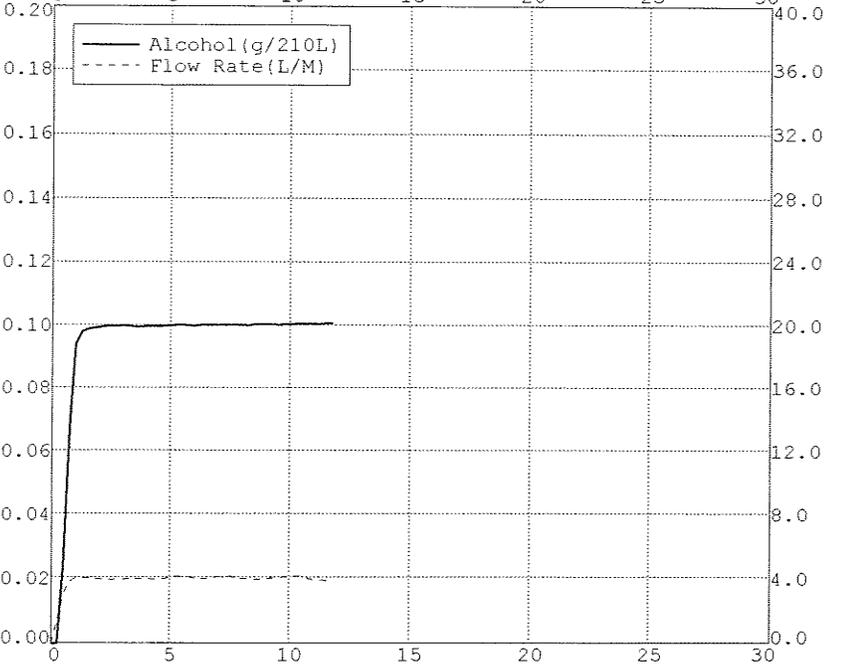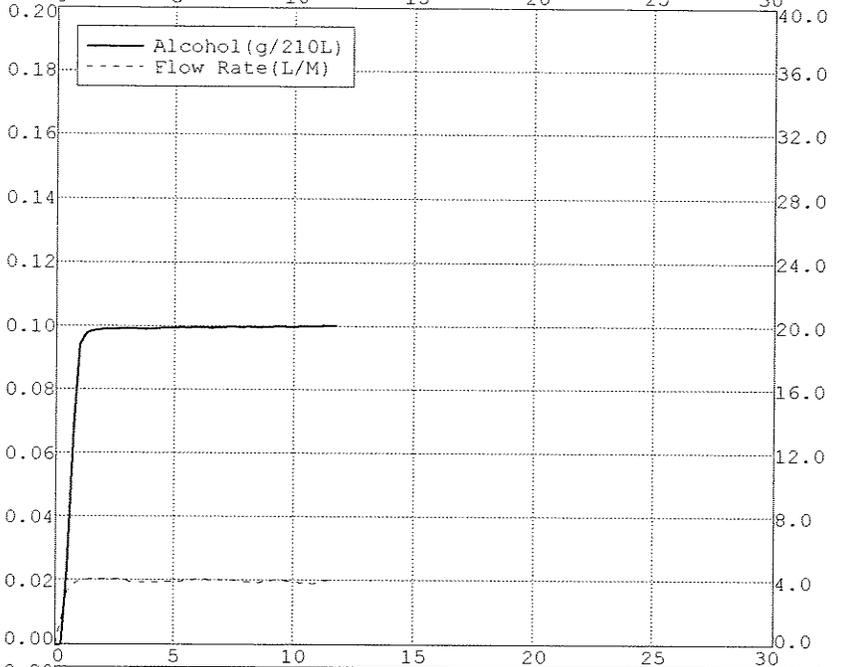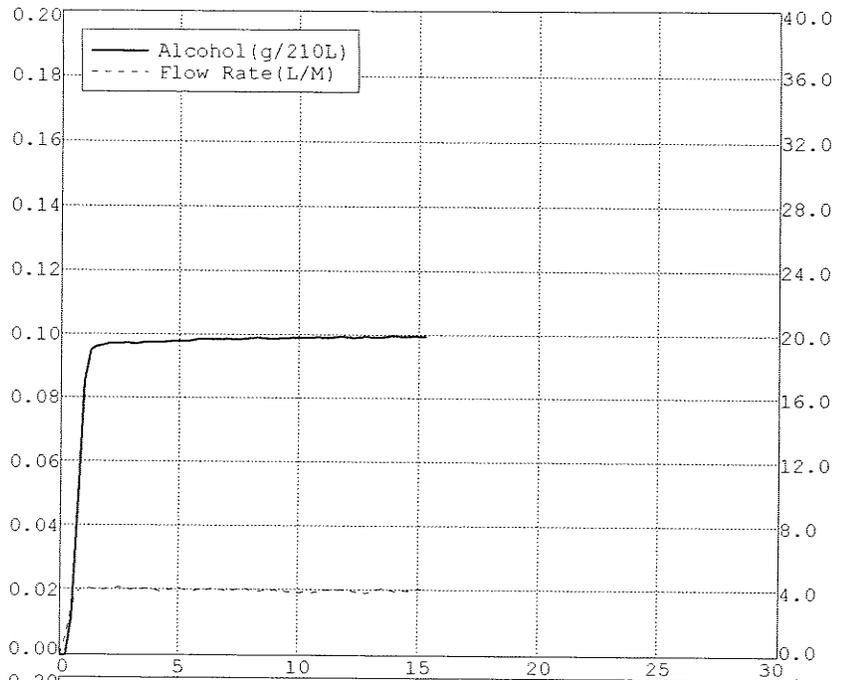

Handwritten signature: C. B. Geisler