

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/01/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:22
INTERNAL STANDARD	VERIFIED	02:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:23
BLANK TEST	0.00	02:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:24
BLANK TEST	0.00	02:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:26
BLANK TEST	0.00	02:27

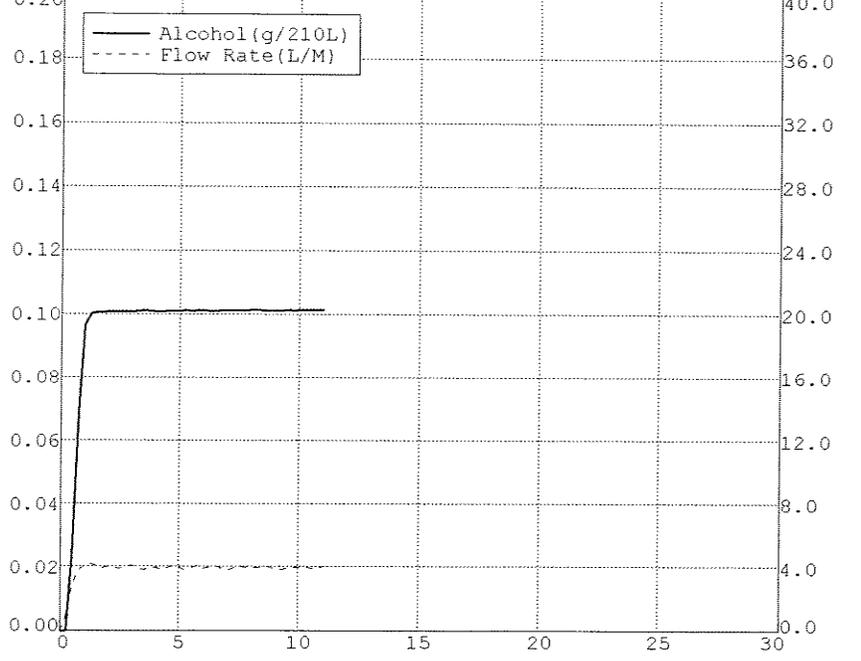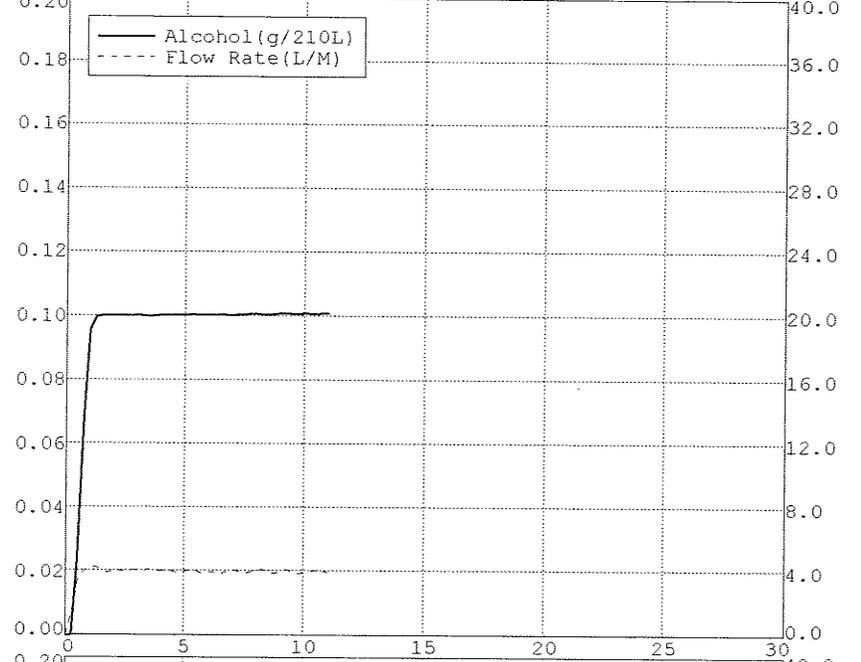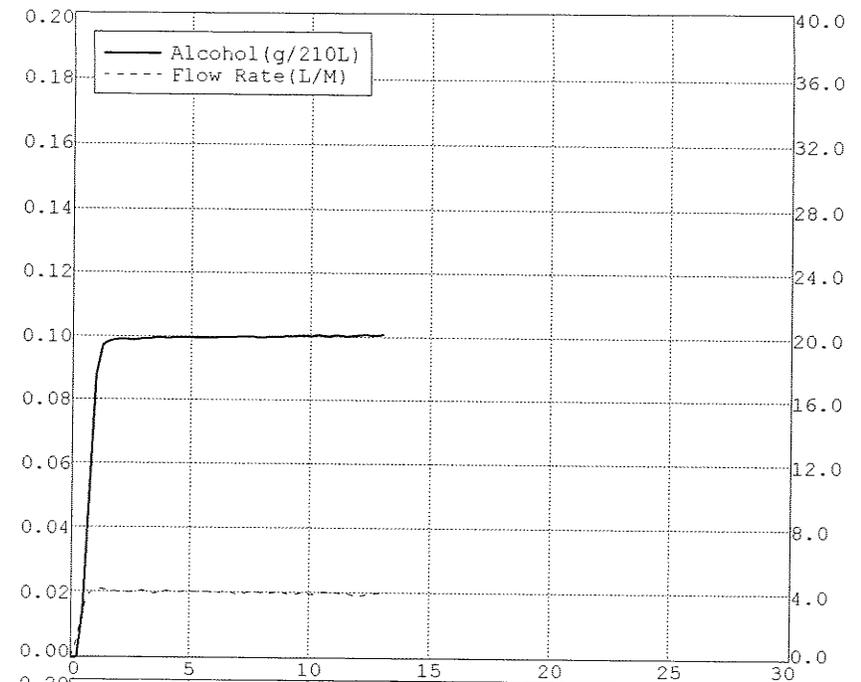

Charles B Geisler