

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/08/2019

OPERATOR NAME:
TYLER J MORSE
Permit #: 41959
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:20
INTERNAL STANDARD	VERIFIED	13:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:21
BLANK TEST	0.00	13:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:22
BLANK TEST	0.00	13:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:24
BLANK TEST	0.00	13:25

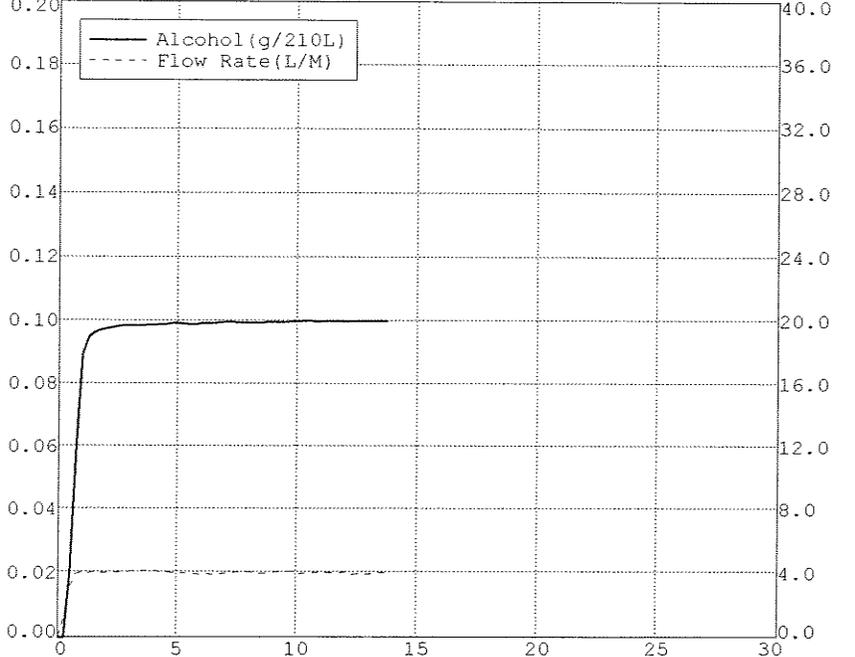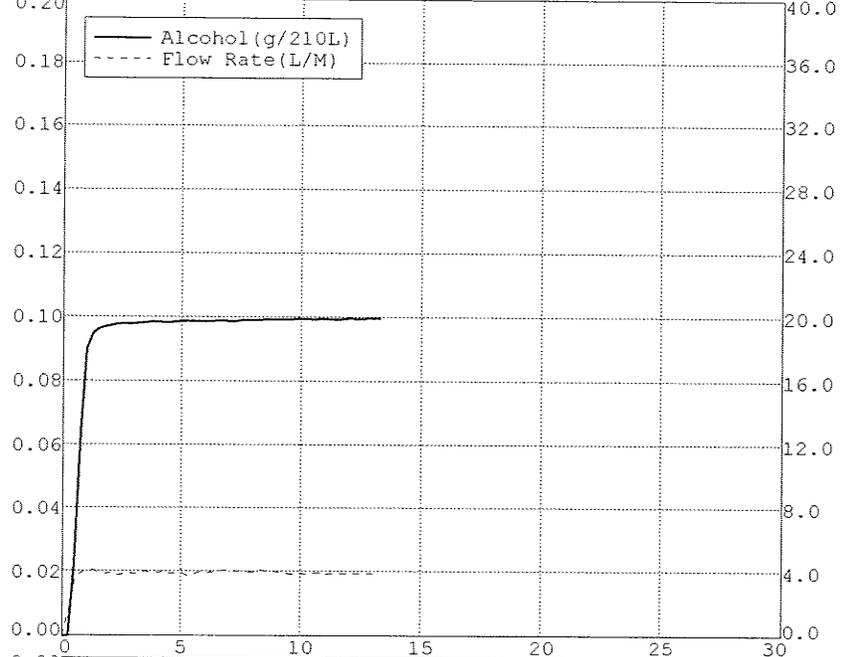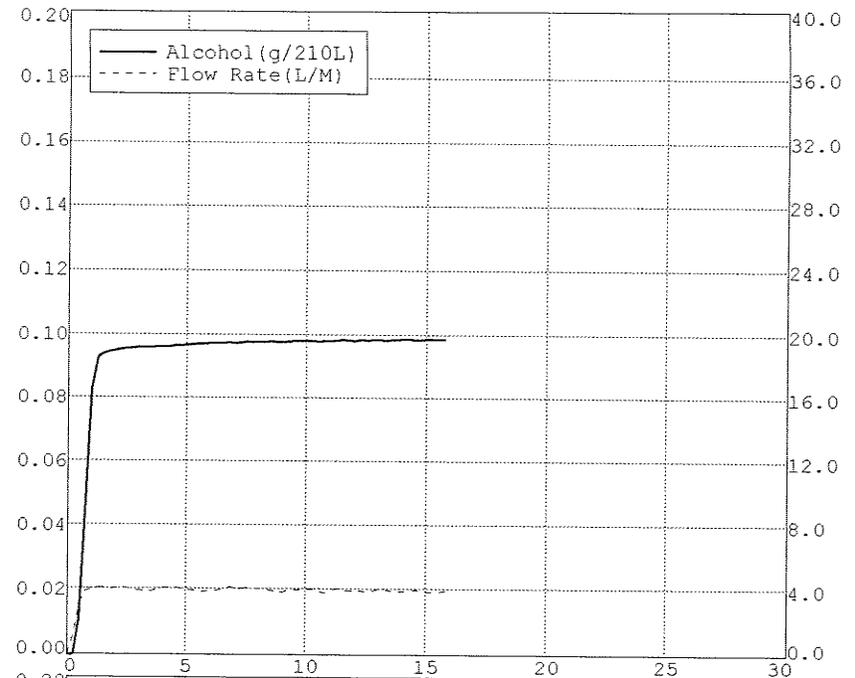

(Handwritten signature)