

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/15/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:49
INTERNAL STANDARD	VERIFIED	01:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:50
BLANK TEST	0.00	01:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:51
BLANK TEST	0.00	01:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:52
BLANK TEST	0.00	01:53

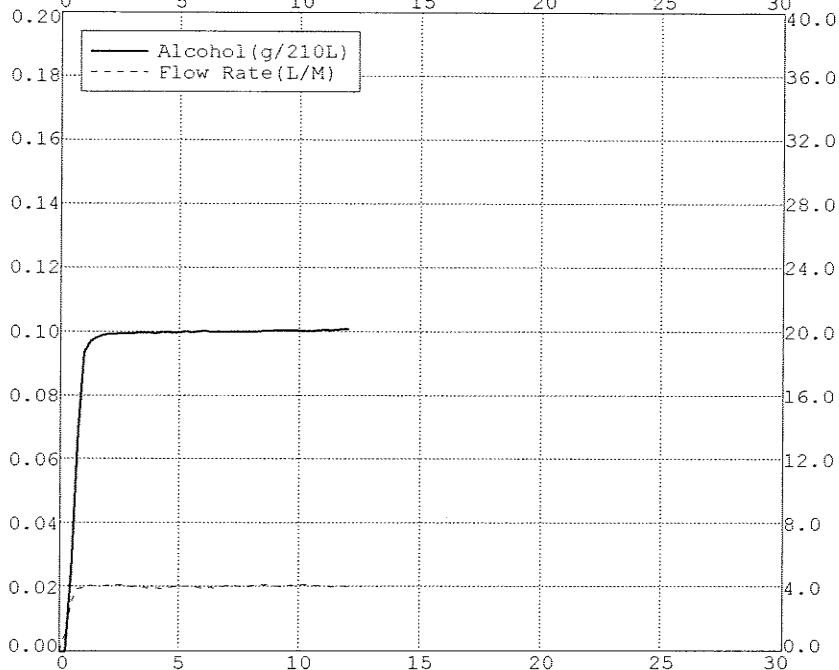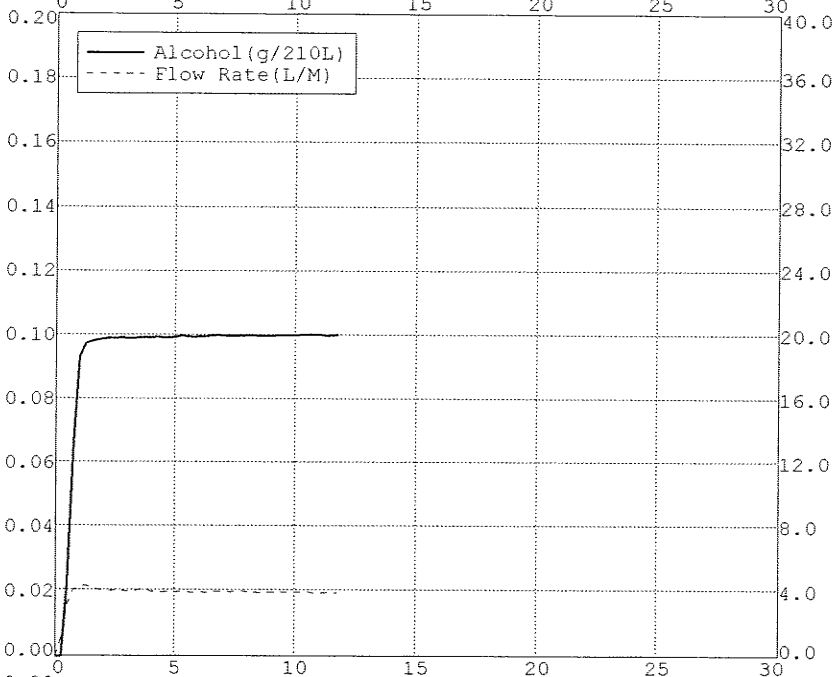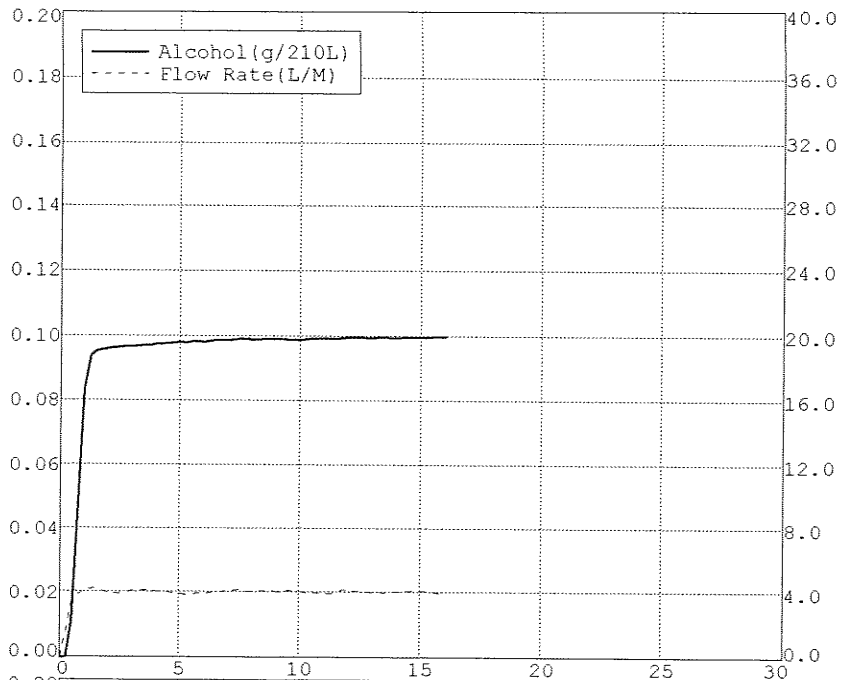

Charles B. Geisler #2W