

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/22/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:33
INTERNAL STANDARD	VERIFIED	23:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:34
BLANK TEST	0.00	23:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:35
BLANK TEST	0.00	23:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:37
BLANK TEST	0.00	23:37

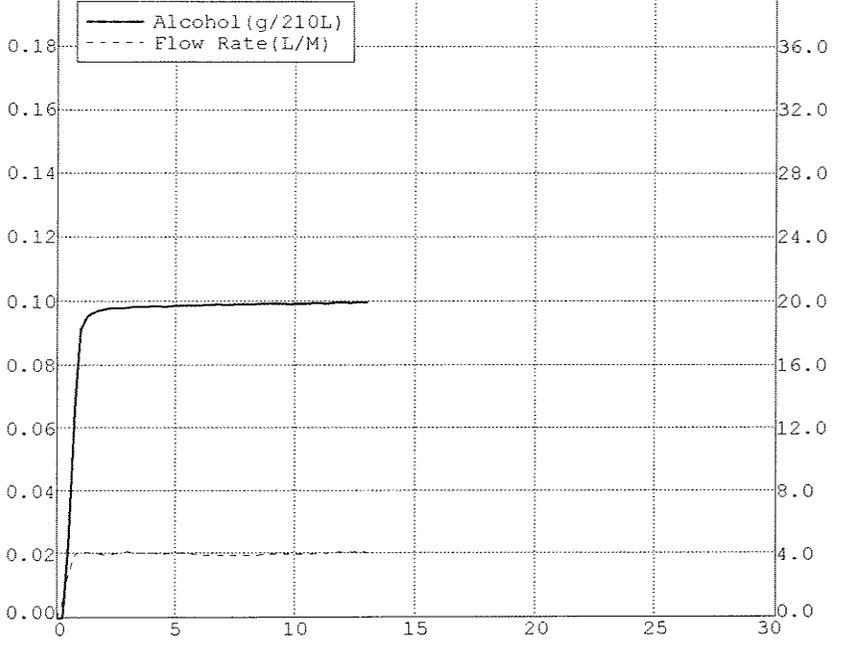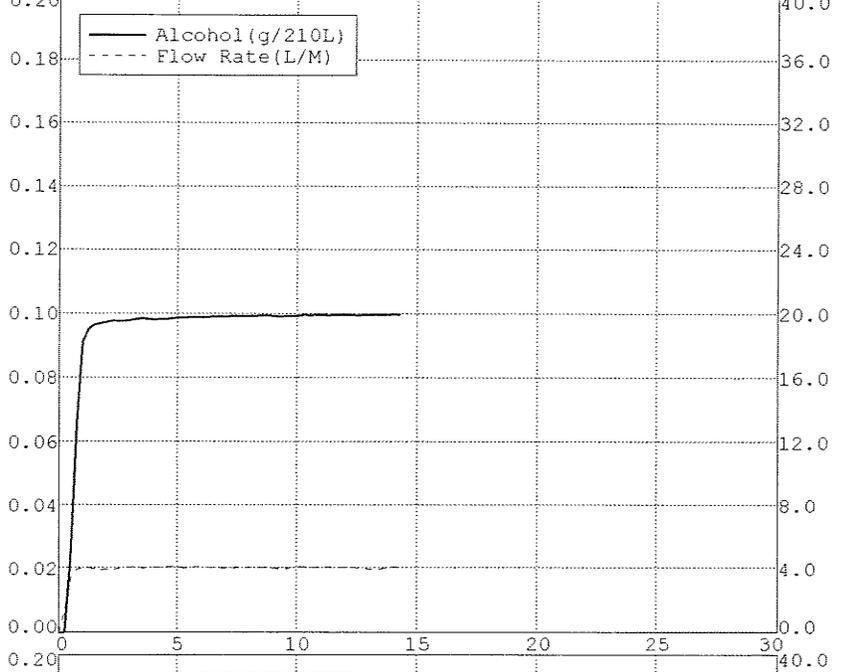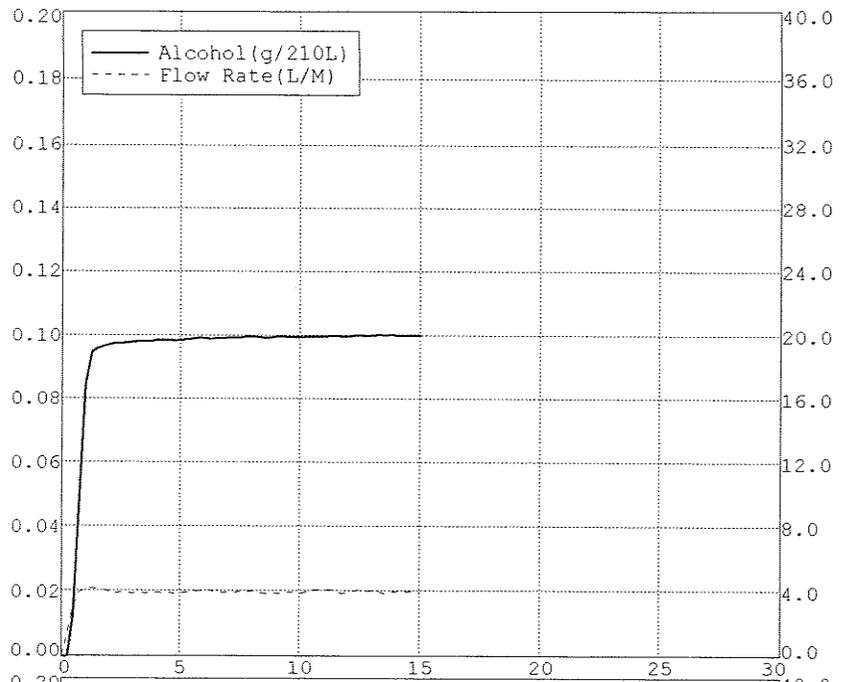

Charles B. Geisler #24