

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/29/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:24
INTERNAL STANDARD	VERIFIED	00:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:25
BLANK TEST	0.00	00:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:26
BLANK TEST	0.00	00:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:27
BLANK TEST	0.00	00:28

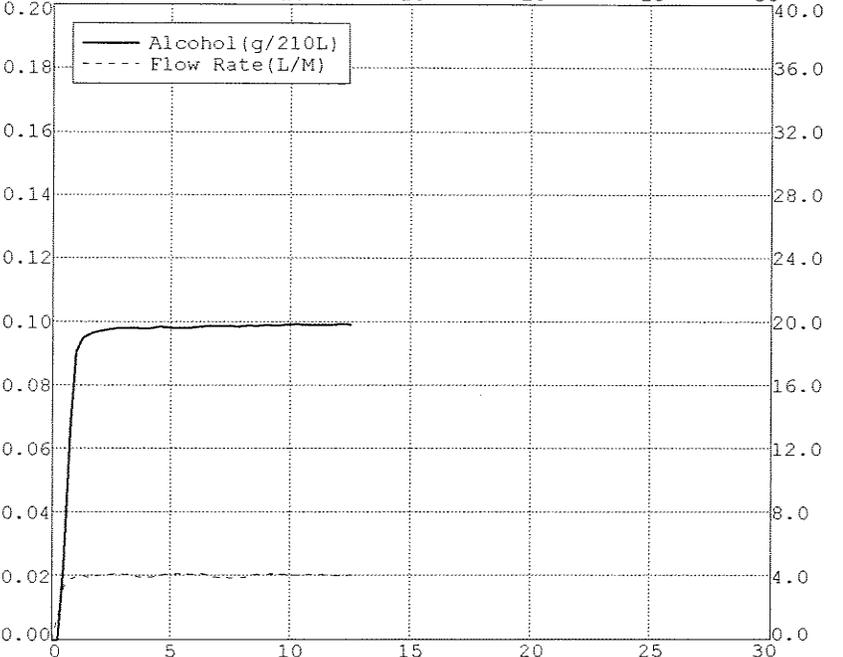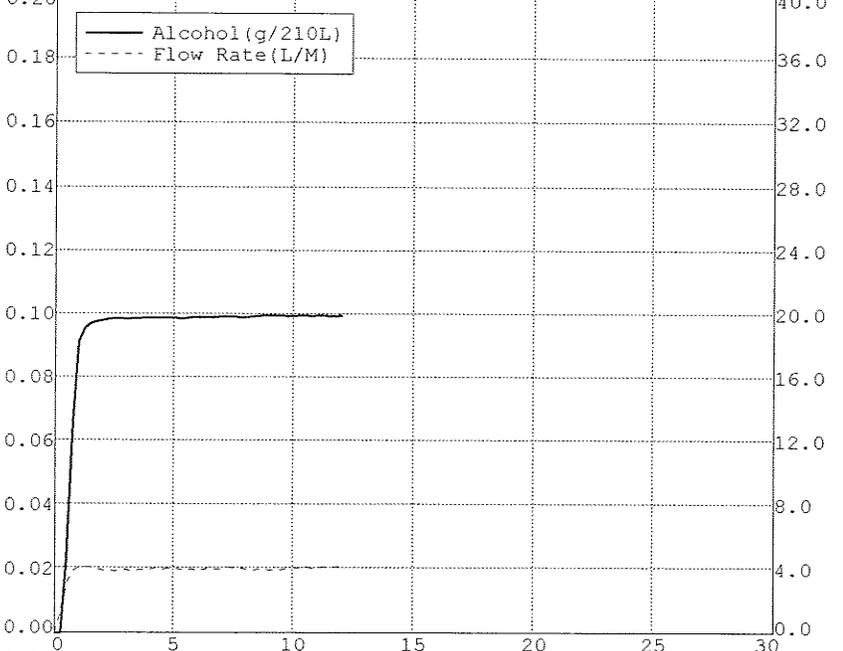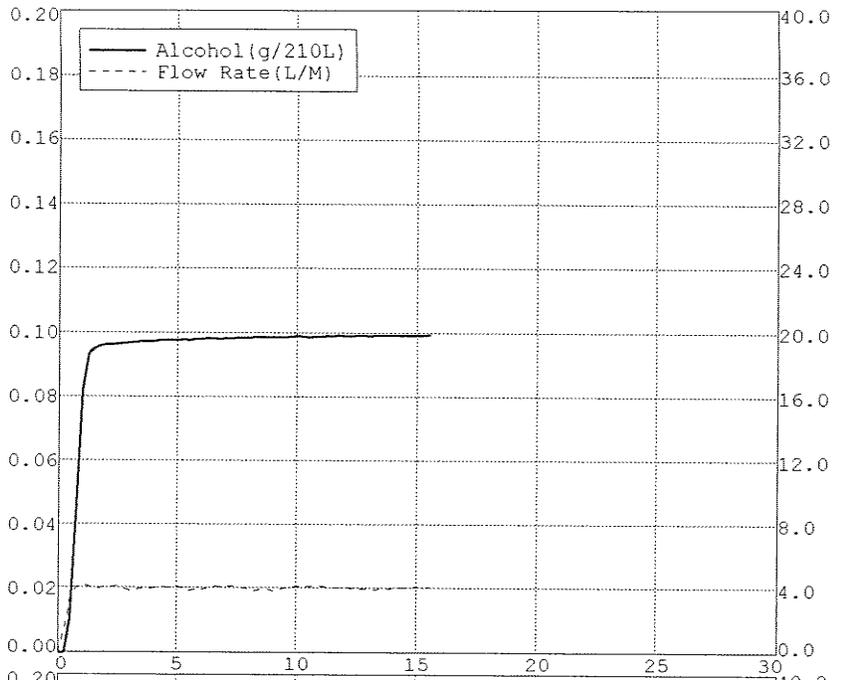

Signature: Charles B. Geisler
#201