

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 08/09/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:31
INTERNAL STANDARD	VERIFIED	22:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:31
BLANK TEST	0.00	22:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:33
BLANK TEST	0.00	22:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:34
BLANK TEST	0.00	22:35

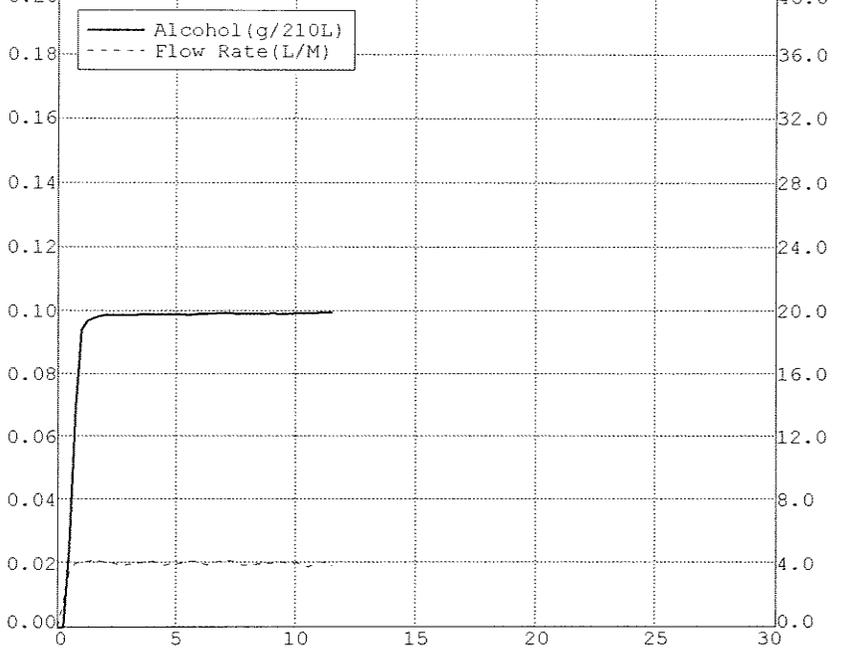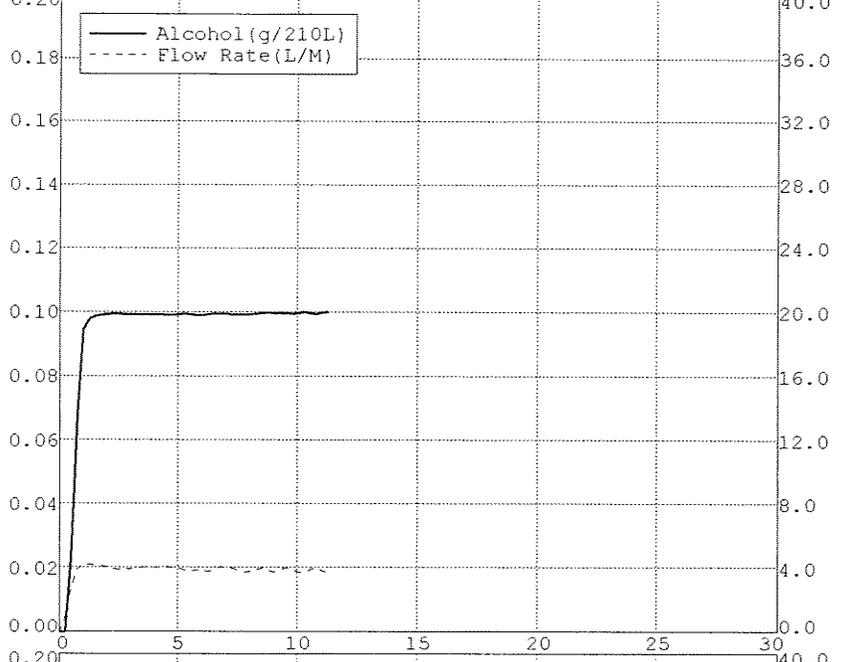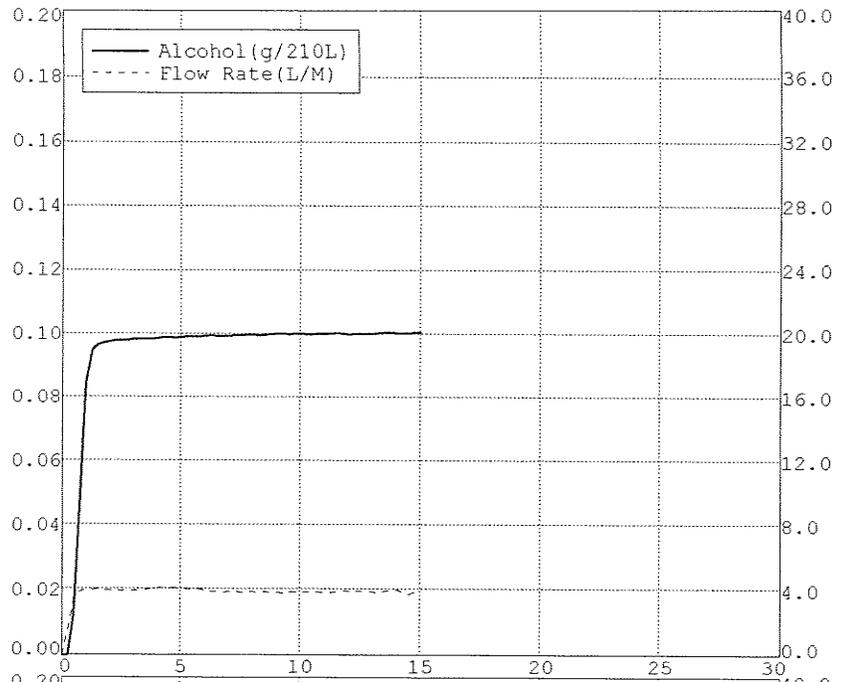

J. B. Geisler