

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 08/20/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:25
INTERNAL STANDARD	VERIFIED	14:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:26
BLANK TEST	0.00	14:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:27
BLANK TEST	0.00	14:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:28
BLANK TEST	0.00	14:29

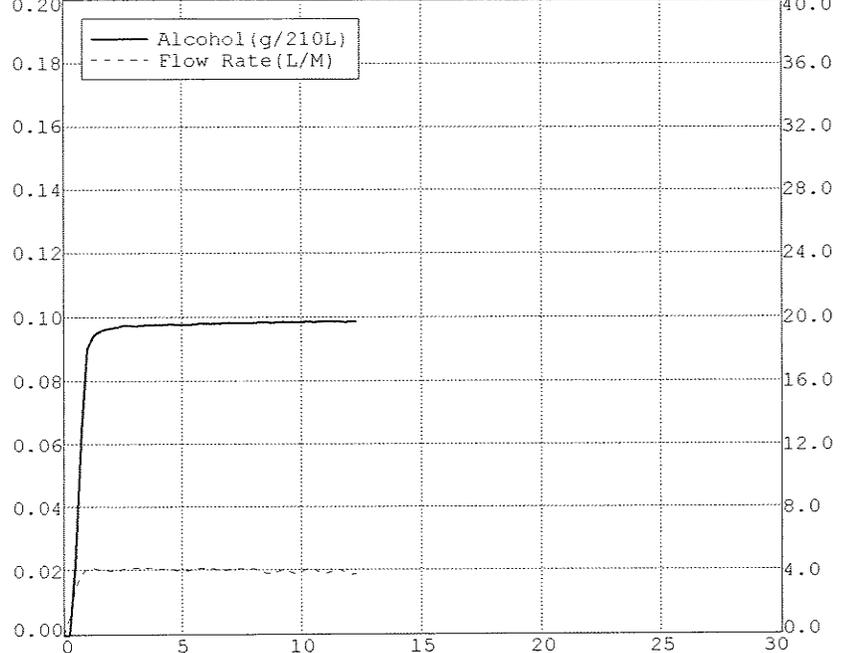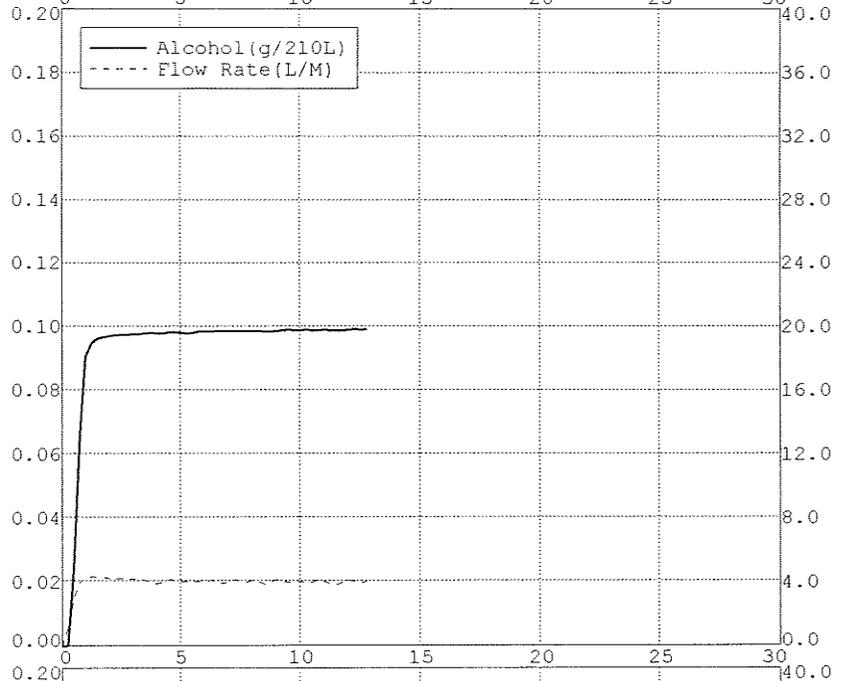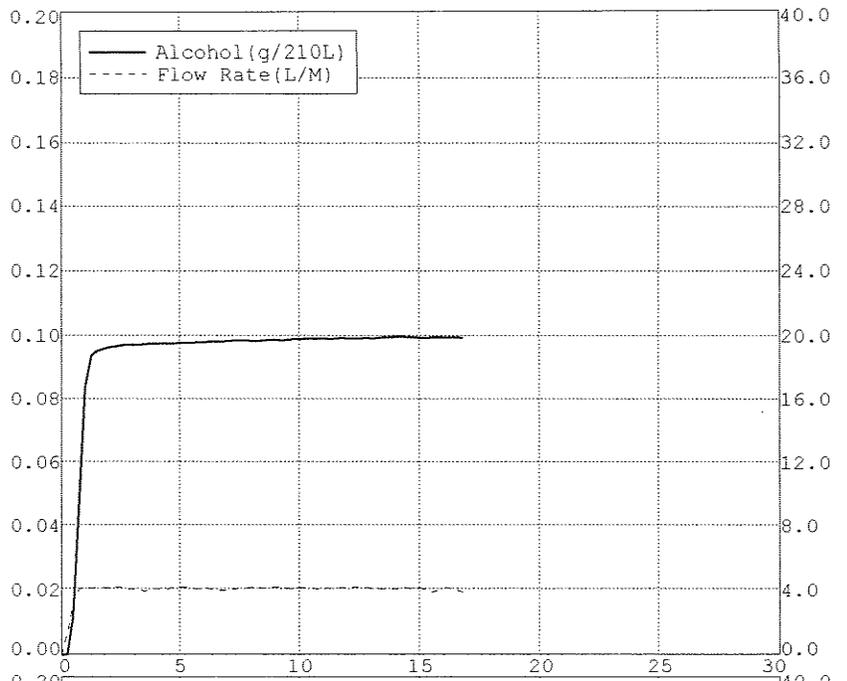

*Handwritten signatures and initials:*  
A. C. B. [Signature] #2