

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 08/27/2019

OPERATOR NAME:
 J T COON
 Permit #: 36043
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:32
INTERNAL STANDARD	VERIFIED	04:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:33
BLANK TEST	0.00	04:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:34
BLANK TEST	0.00	04:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	04:35
BLANK TEST	0.00	04:36

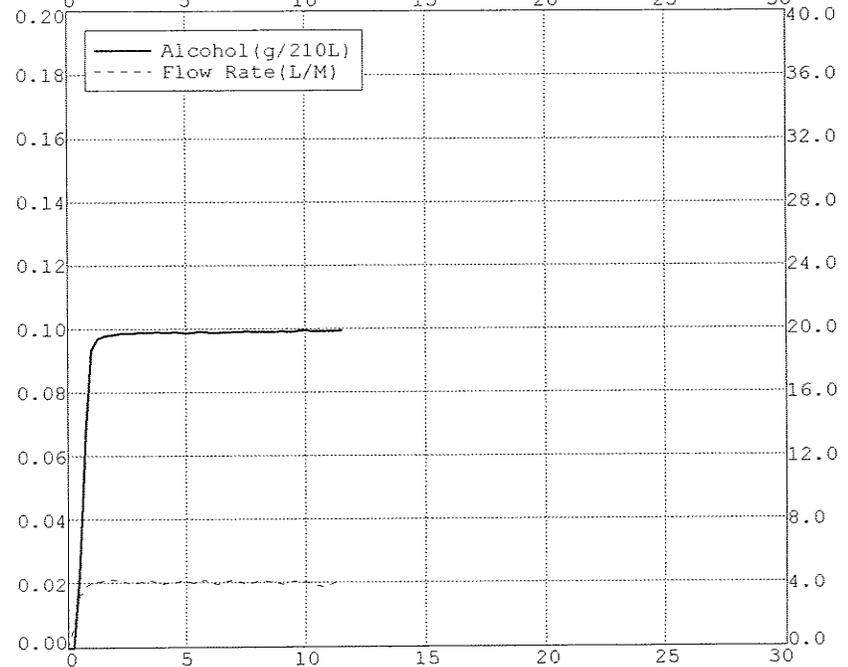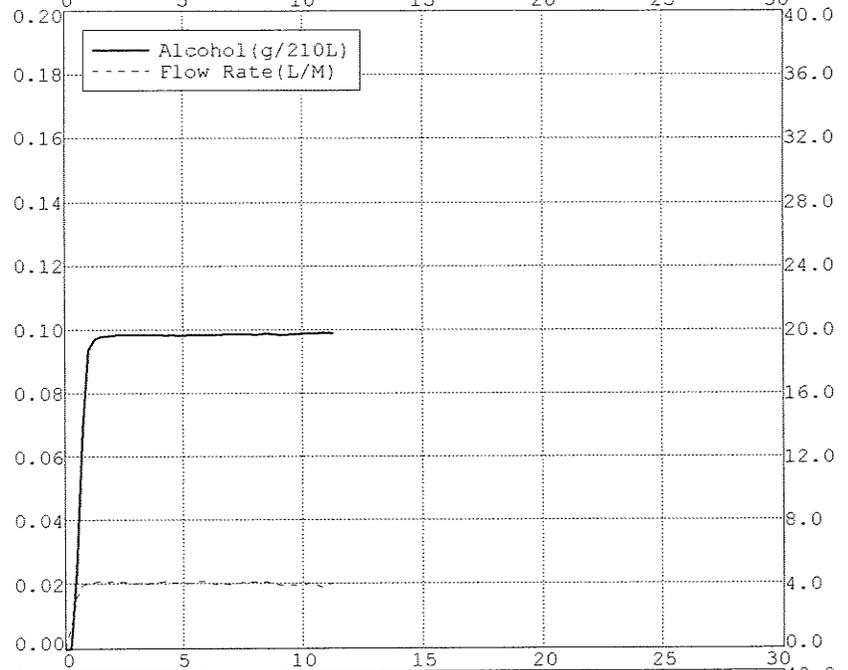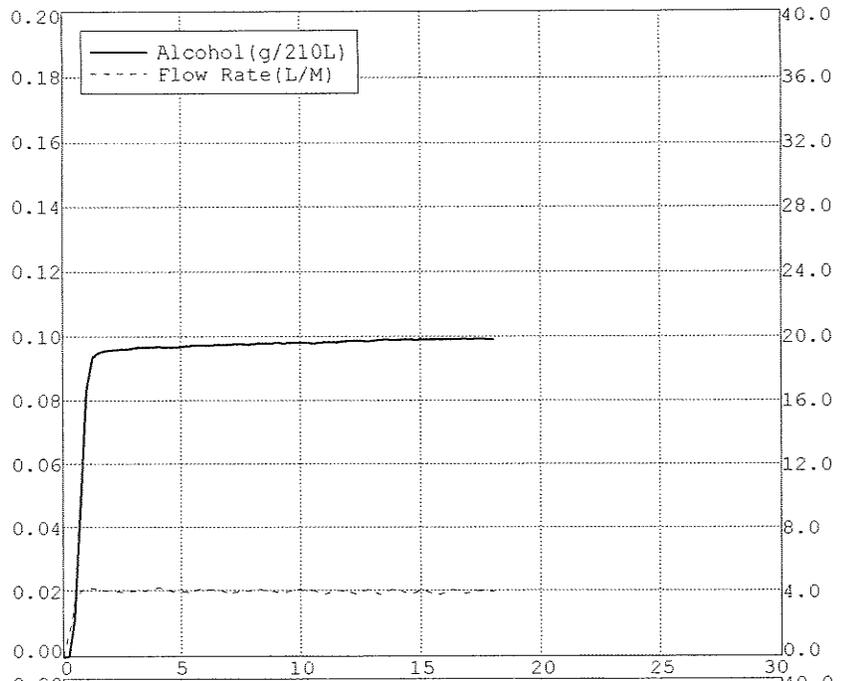

P.O. *[Signature]* 341