

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 09/09/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:19
INTERNAL STANDARD	VERIFIED	05:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	05:19
BLANK TEST	0.00	05:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:21
BLANK TEST	0.00	05:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:22
BLANK TEST	0.00	05:23

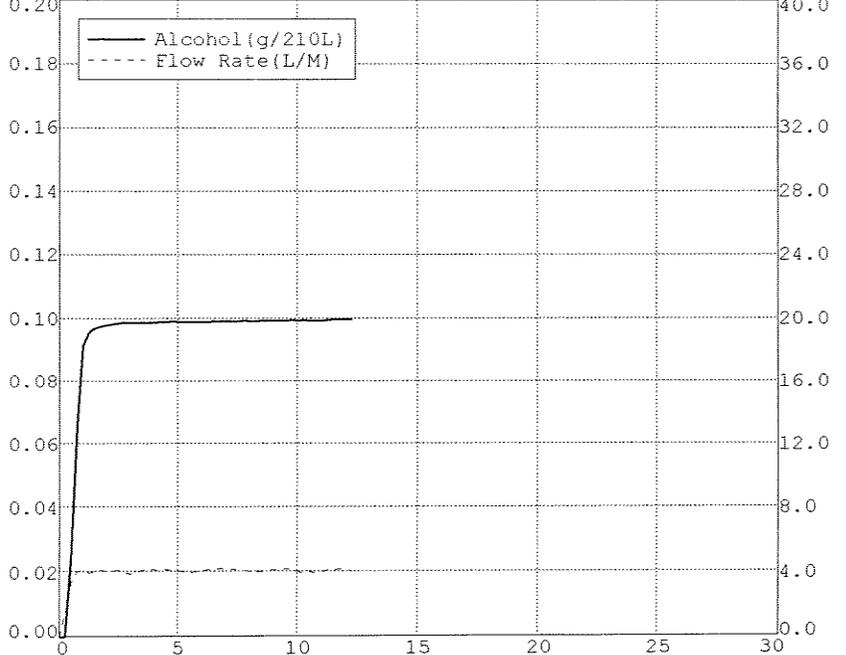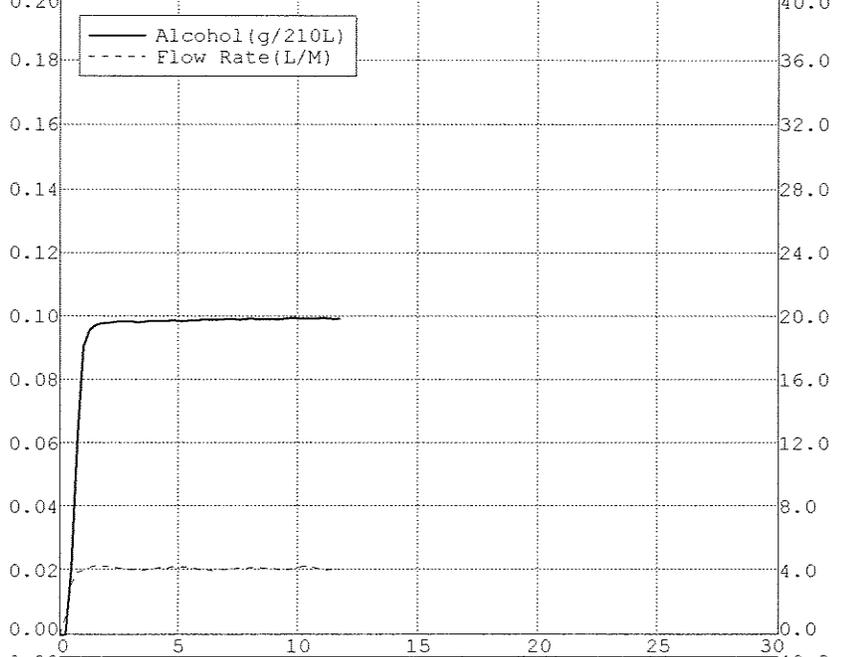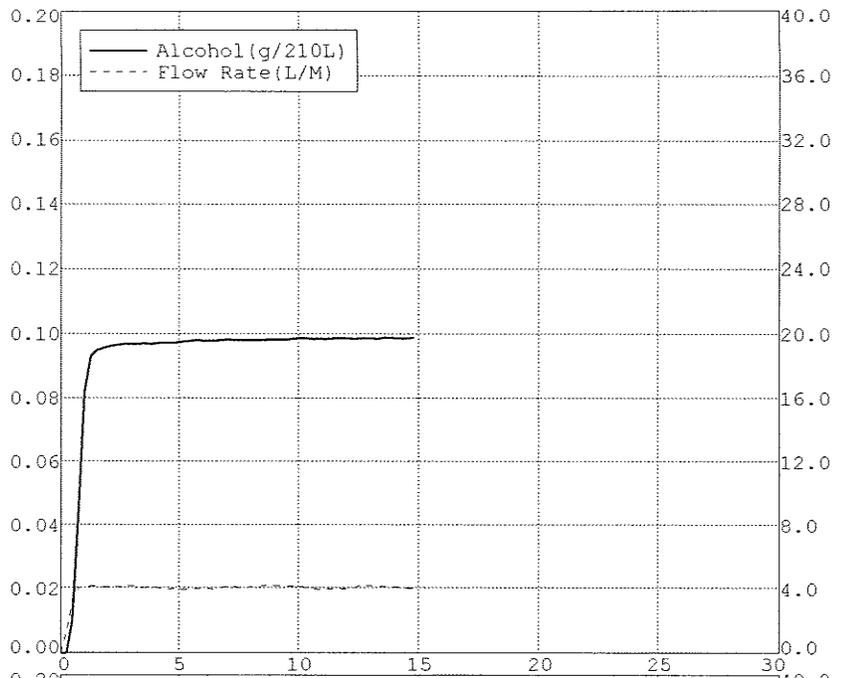

Charles B. Geisler #248