

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 09/21/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:26
INTERNAL STANDARD	VERIFIED	05:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	05:26
BLANK TEST	0.00	05:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	05:28
BLANK TEST	0.00	05:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:29
BLANK TEST	0.00	05:30

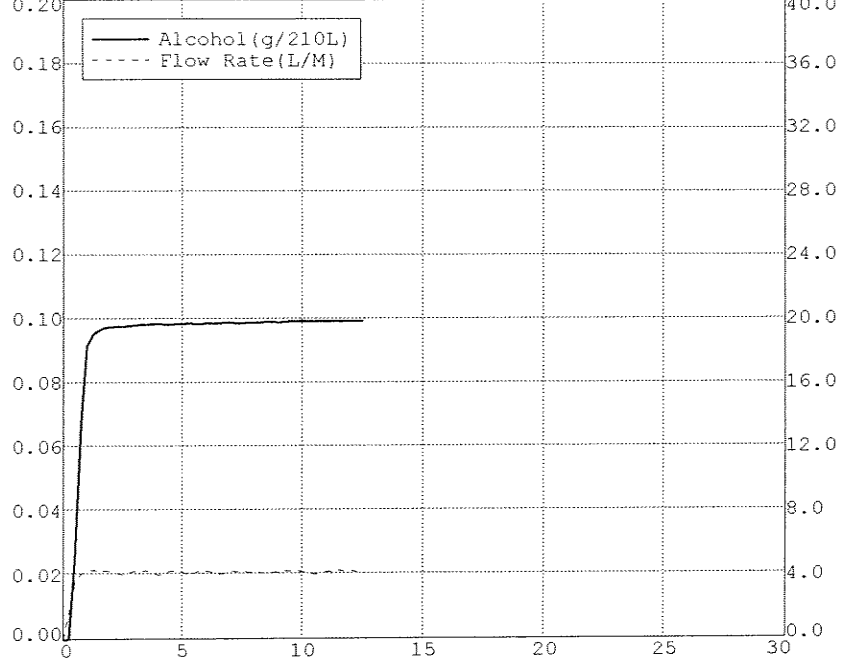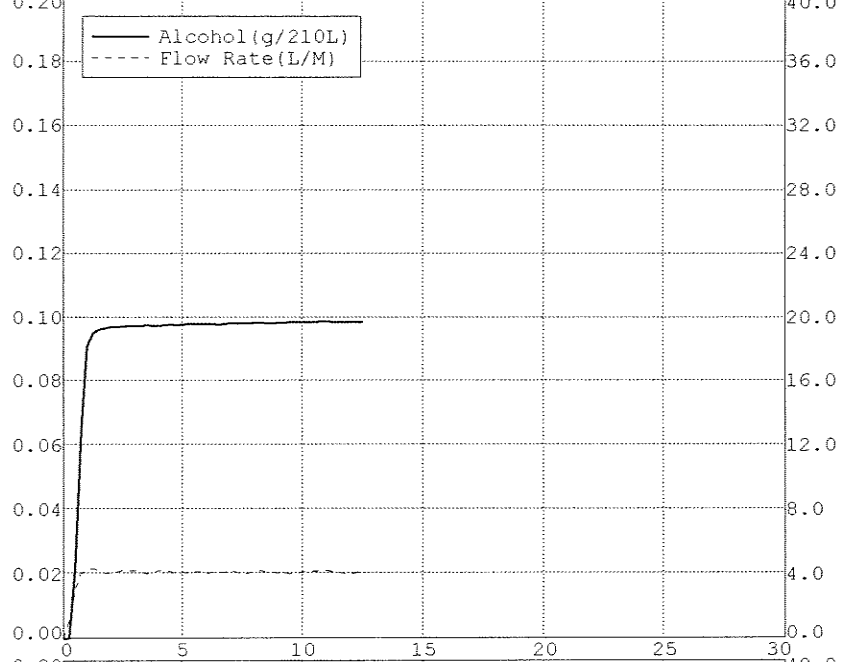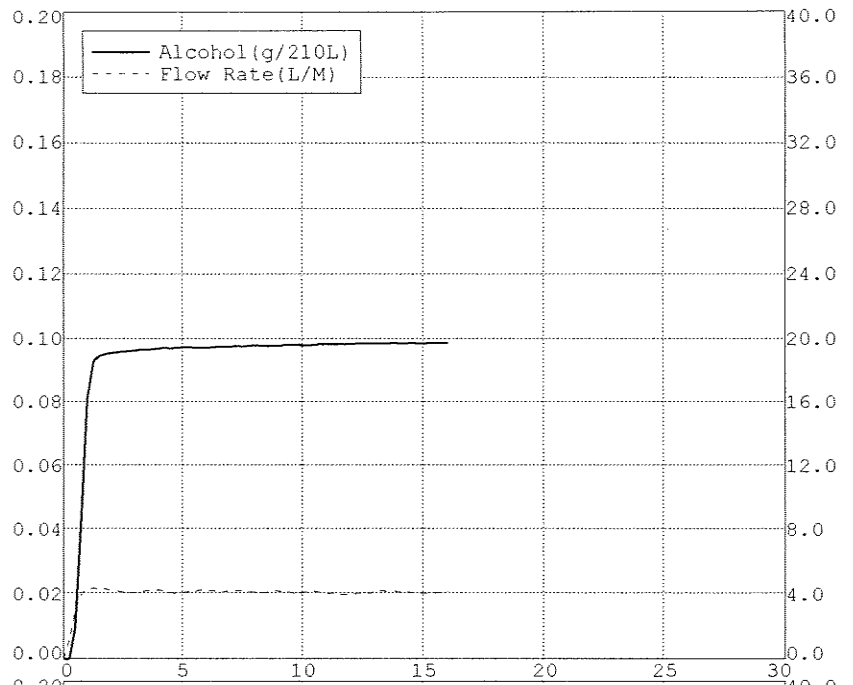

*Handwritten signature: Sgt. Charles B. Geisler*