

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 10/09/2019

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:27
INTERNAL STANDARD	VERIFIED	12:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:27
BLANK TEST	0.00	12:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:28
BLANK TEST	0.00	12:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:30
BLANK TEST	0.00	12:30

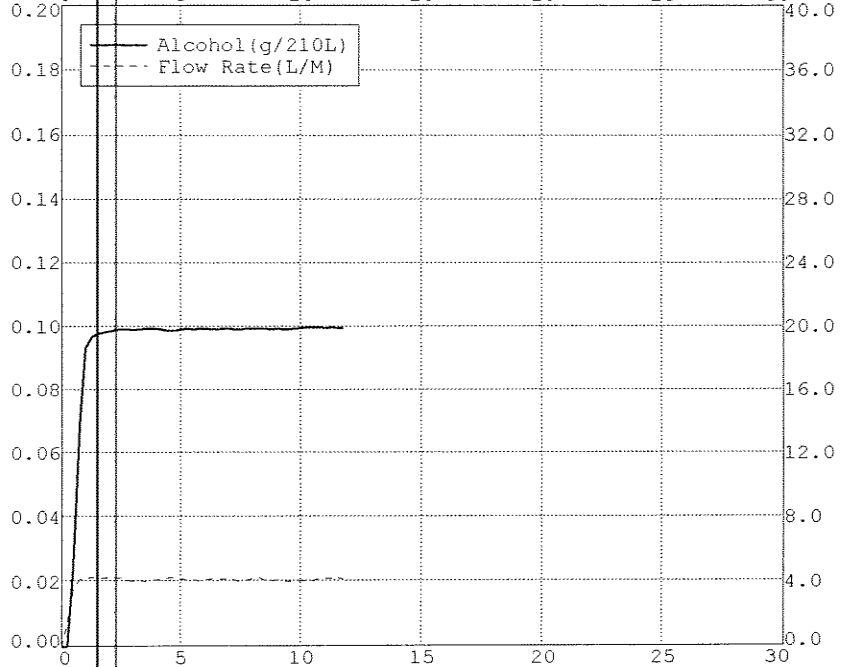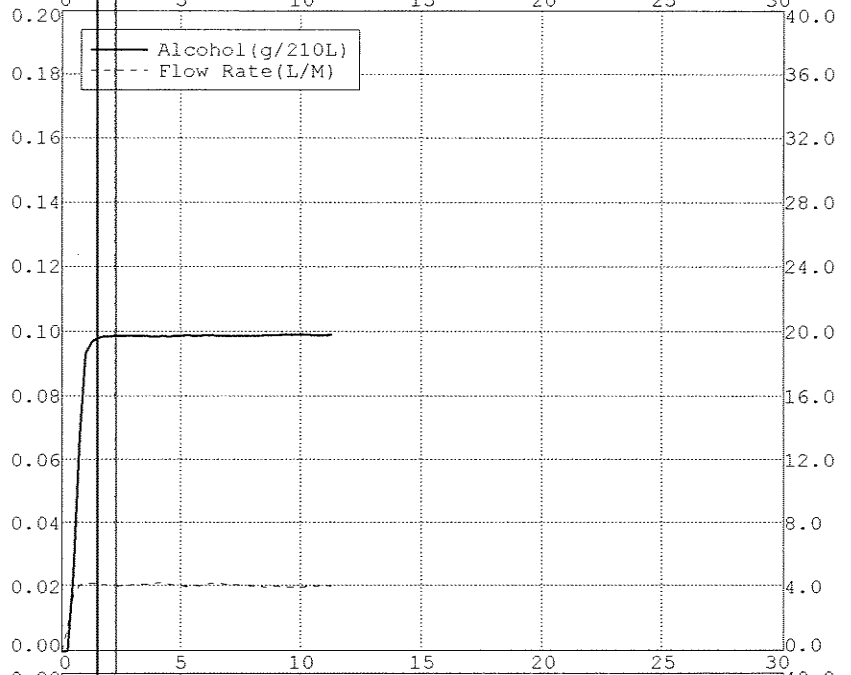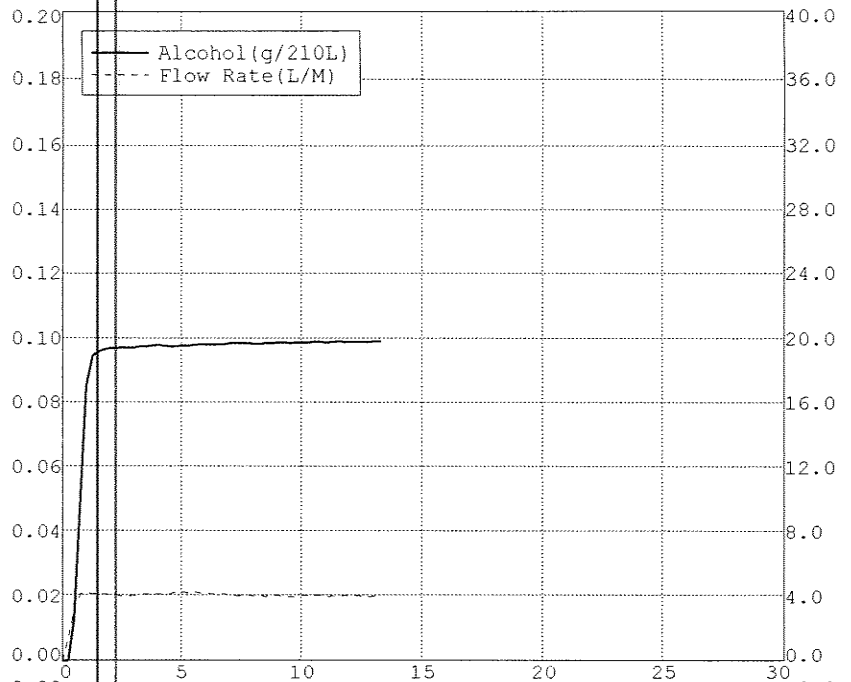

Charles B Geisler