

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 10/30/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:08
INTERNAL STANDARD	VERIFIED	03:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:09
BLANK TEST	0.00	03:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:10
BLANK TEST	0.00	03:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:11
BLANK TEST	0.00	03:12

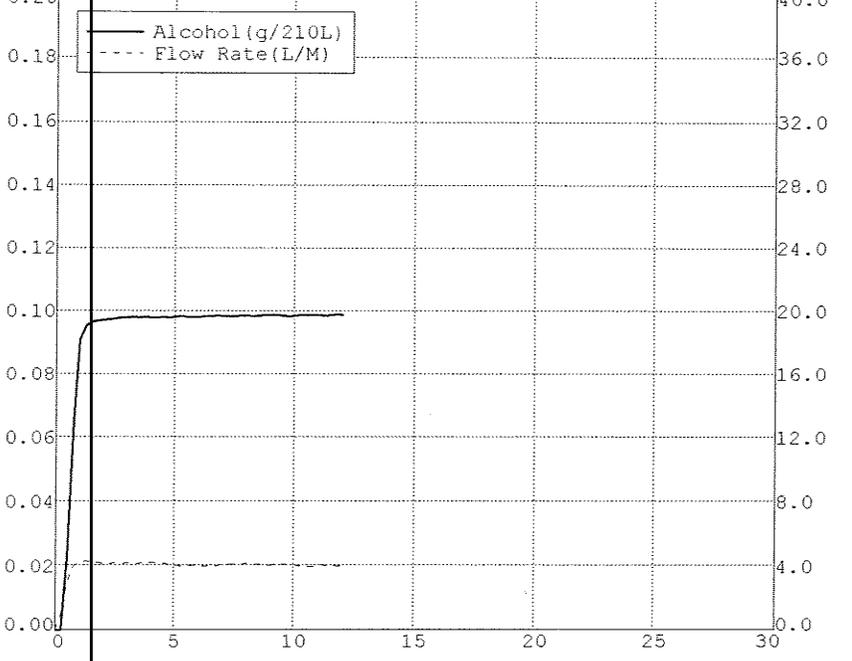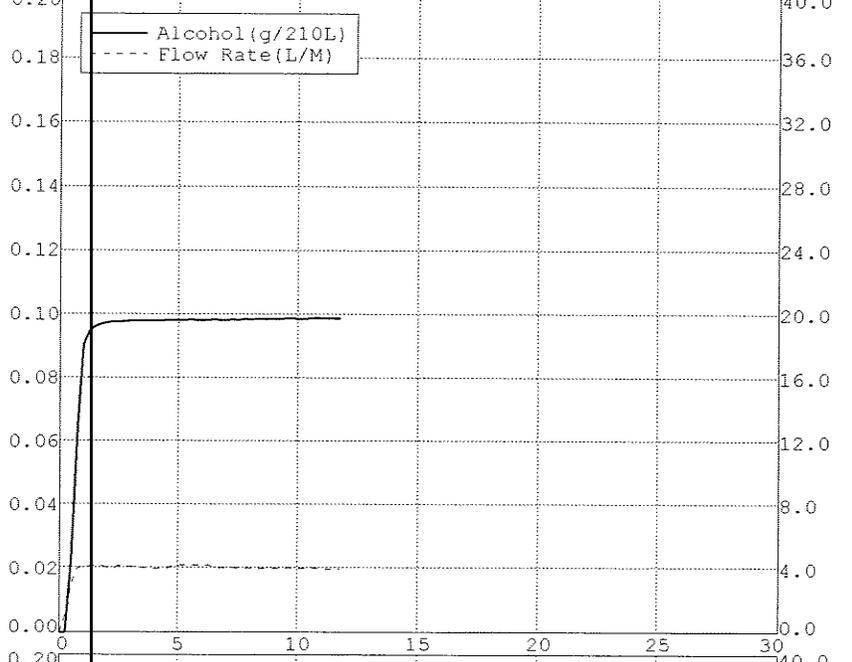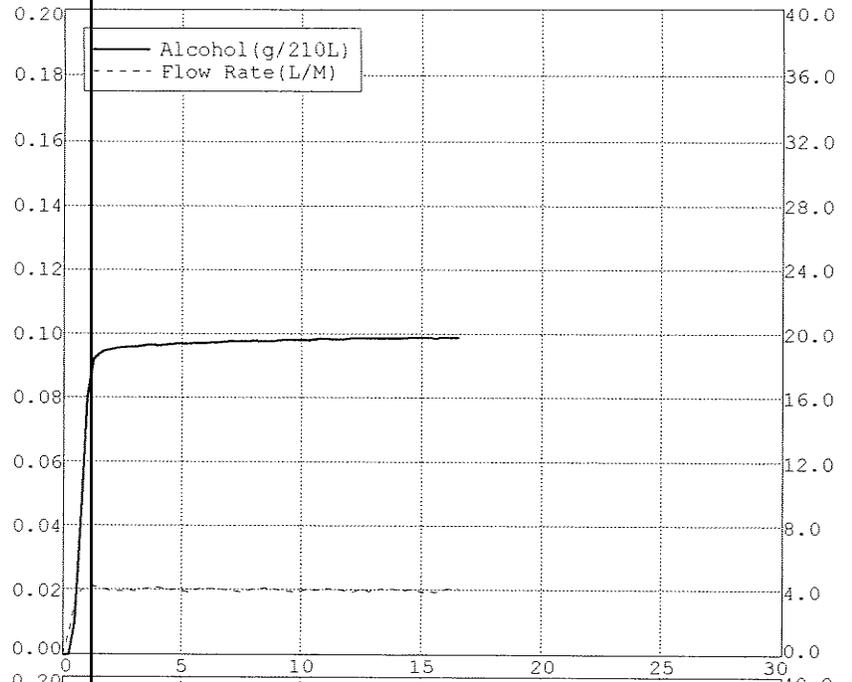

Sgt. Charles B. Geisler