

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/07/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:06
INTERNAL STANDARD	VERIFIED	12:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:06
BLANK TEST	0.00	12:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:08
BLANK TEST	0.00	12:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:09
BLANK TEST	0.00	12:10

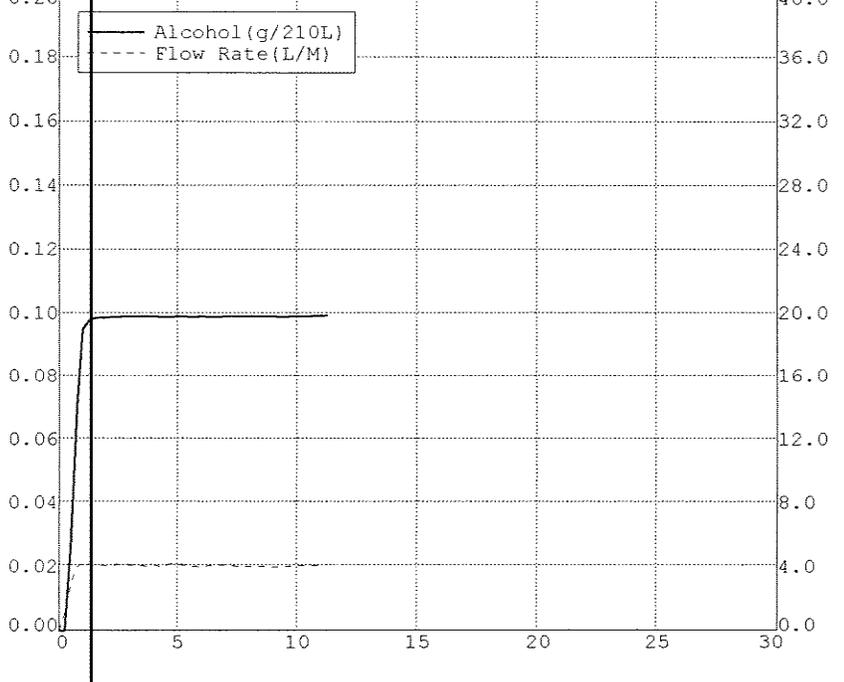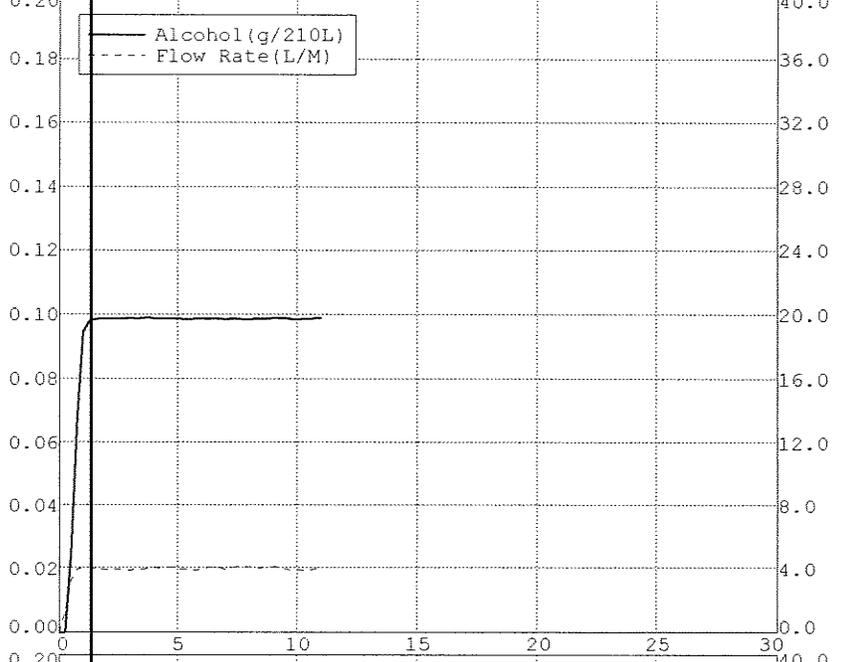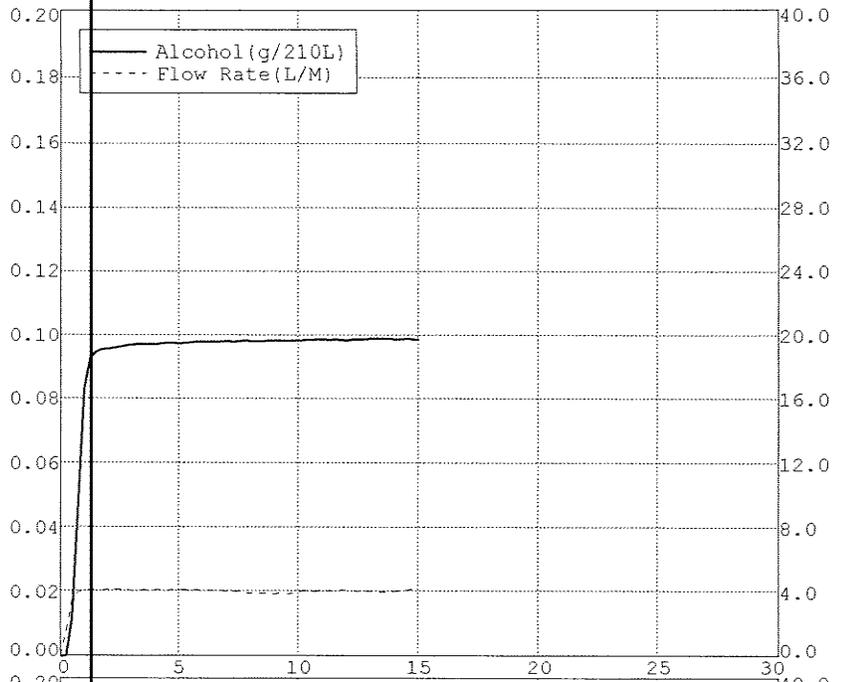

Charles B. Geisler *[Signature]*