

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/15/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:28
INTERNAL STANDARD	VERIFIED	23:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:29
BLANK TEST	0.00	23:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:30
BLANK TEST	0.00	23:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:31
BLANK TEST	0.00	23:32

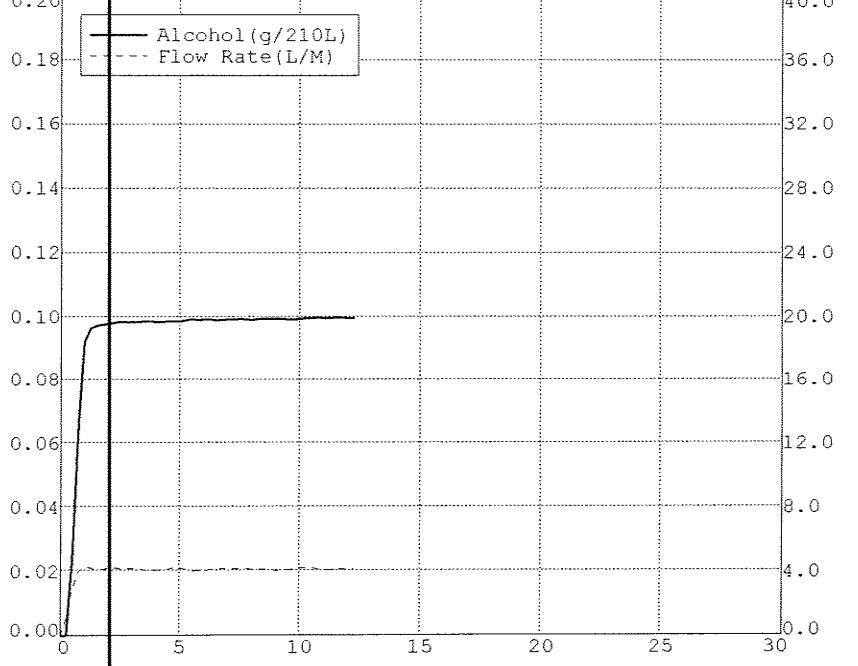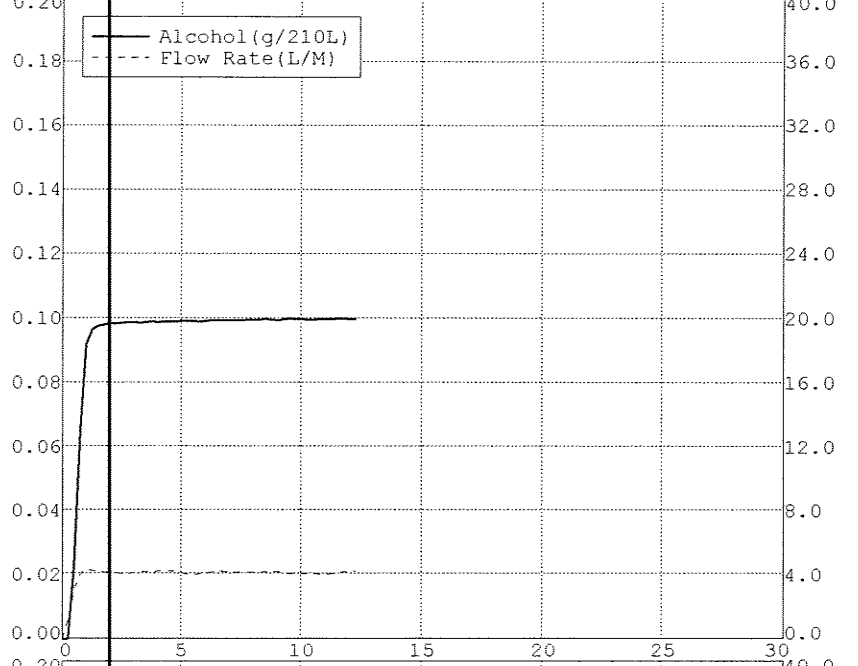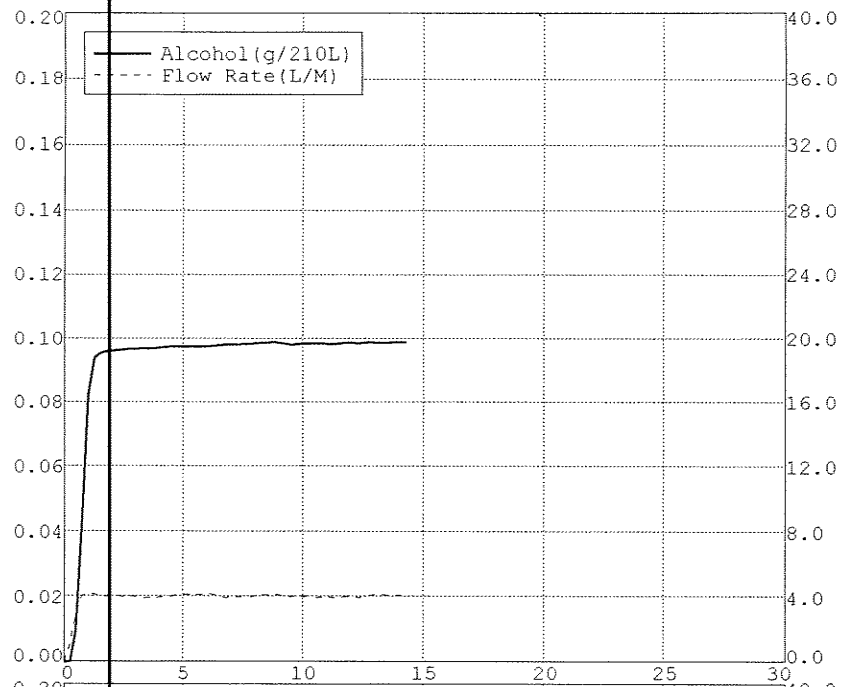

Charles B. Geisler #2011