

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/01/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:13
INTERNAL STANDARD	VERIFIED	00:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:13
BLANK TEST	0.00	00:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:15
BLANK TEST	0.00	00:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:16
BLANK TEST	0.00	00:17

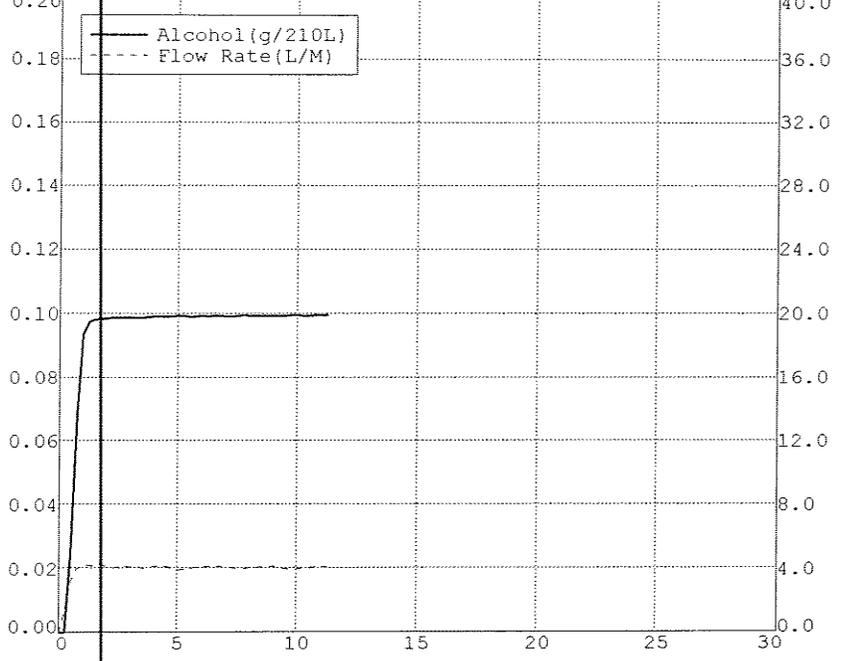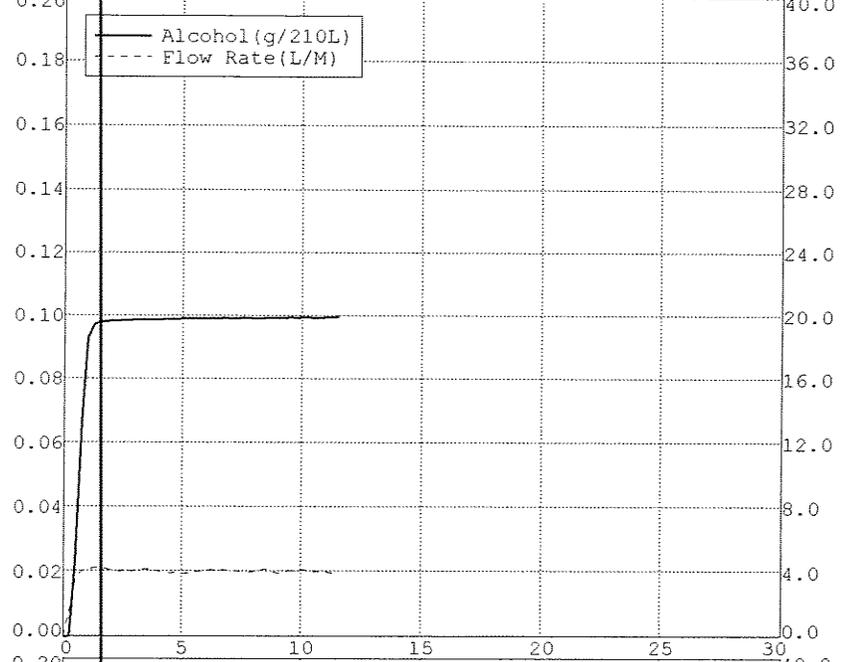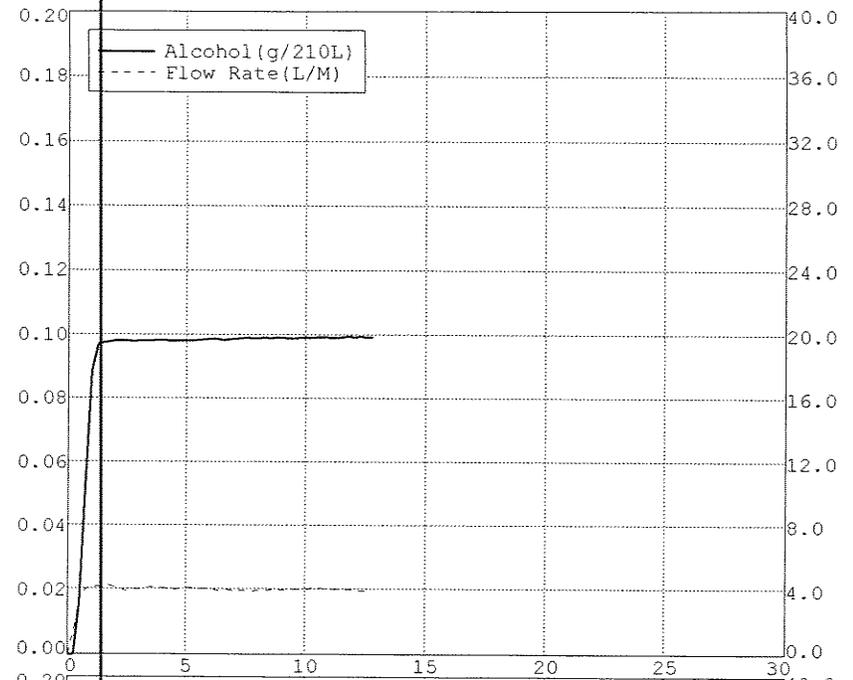

Charles B. Geisler