

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 12/06/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:45
INTERNAL STANDARD	VERIFIED	02:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:46
BLANK TEST	0.00	02:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:47
BLANK TEST	0.00	02:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:48
BLANK TEST	0.00	02:49

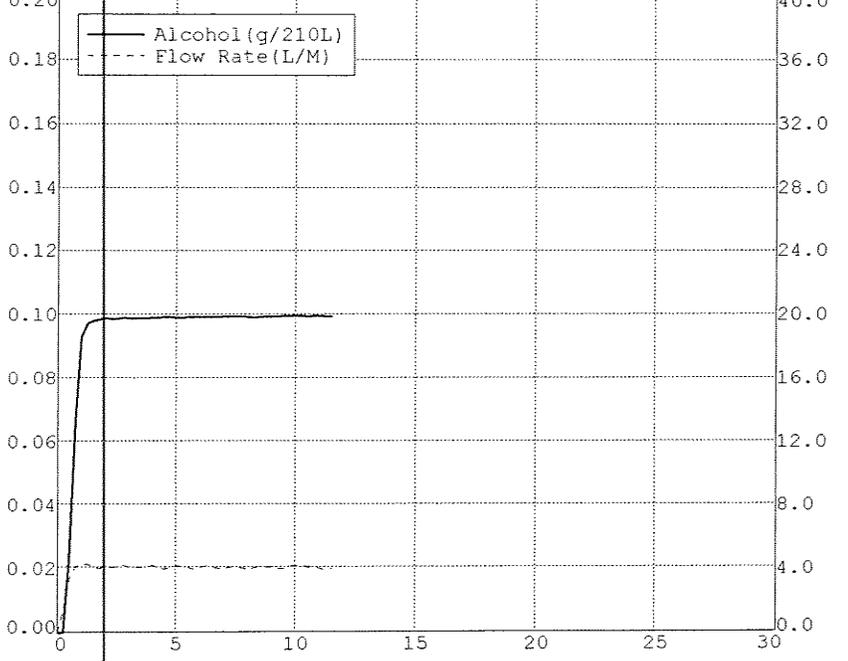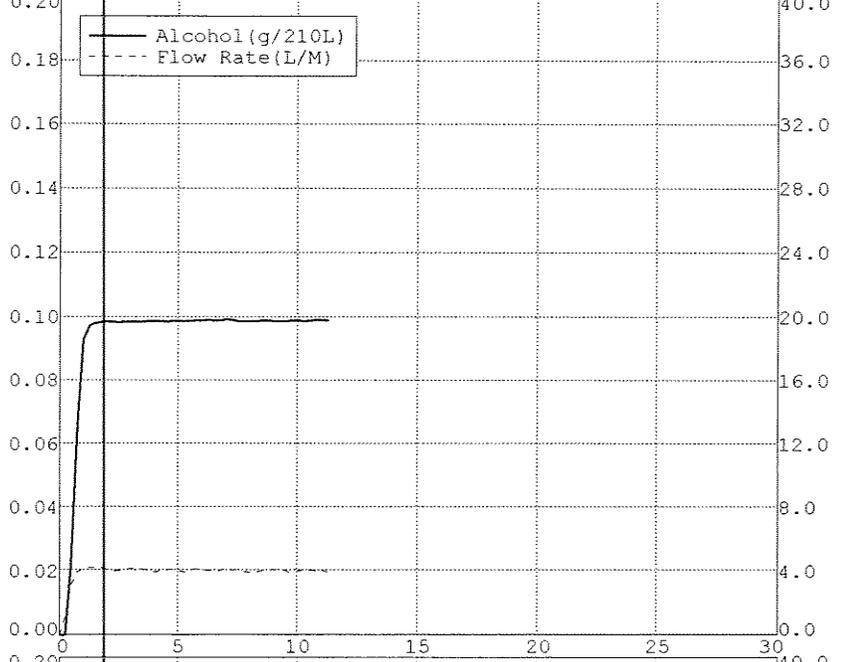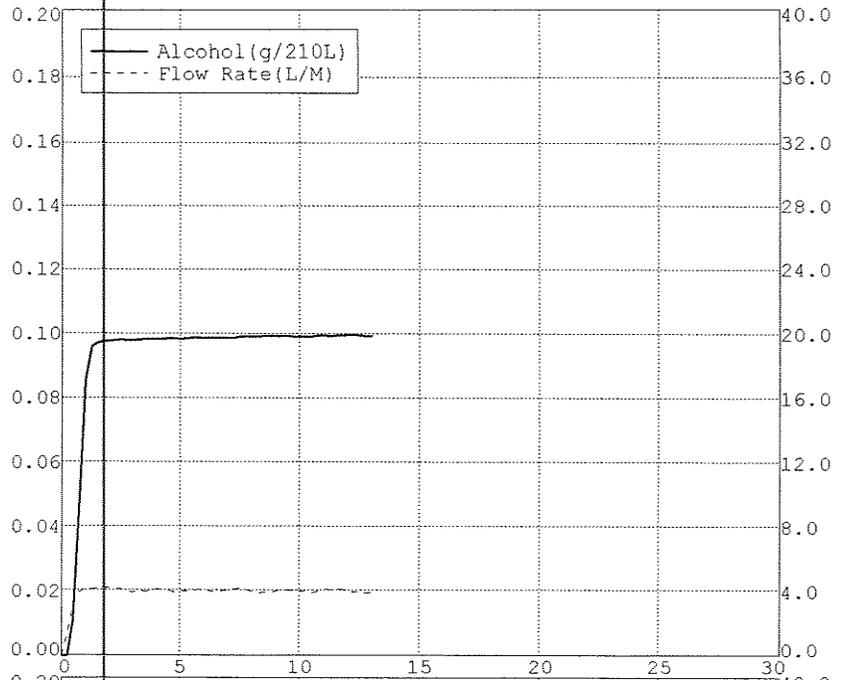

*Charles B. Geisler #241*