

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/14/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:21
INTERNAL STANDARD	VERIFIED	05:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:22
BLANK TEST	0.00	05:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	05:23
BLANK TEST	0.00	05:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:24
BLANK TEST	0.00	05:25

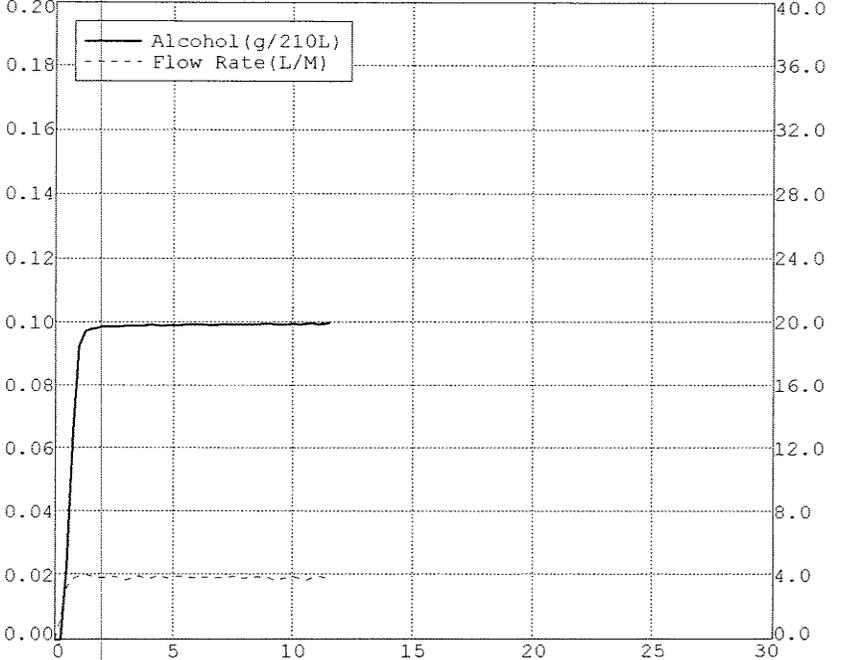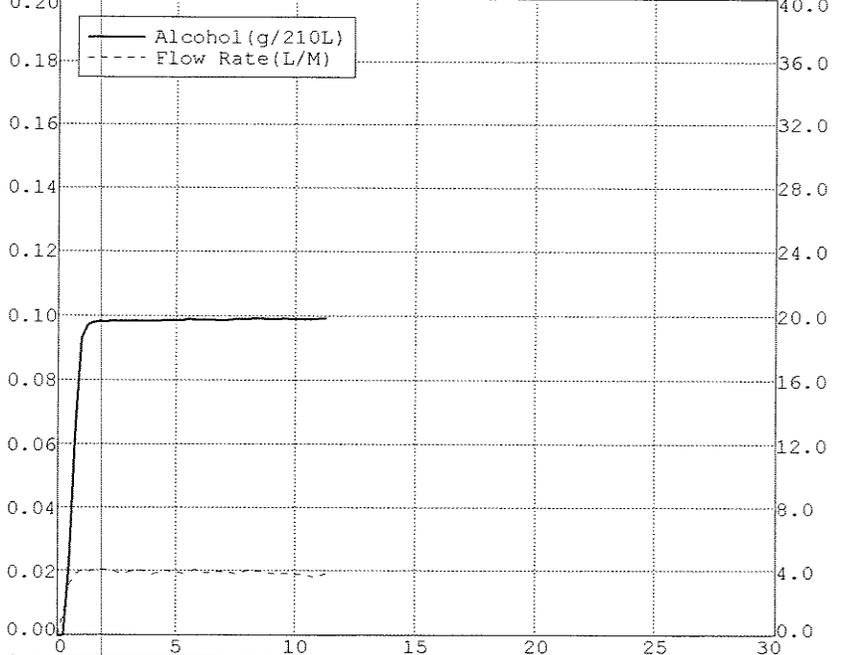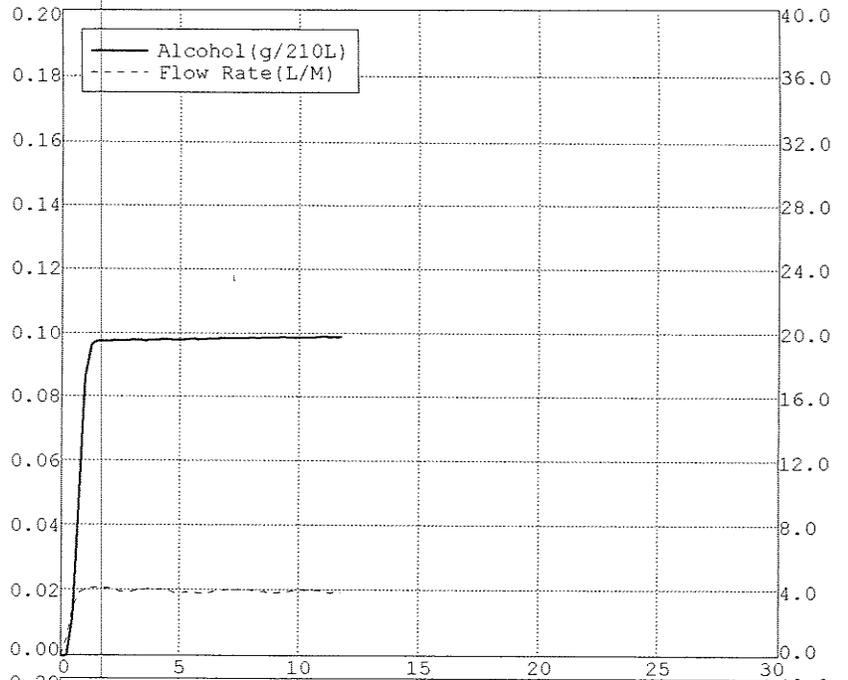

Charles B. Geisler #241