

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/02/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:58
INTERNAL STANDARD	VERIFIED	19:58
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	19:59
BLANK TEST	0.00	19:59
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	20:00
BLANK TEST	0.00	20:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:01
BLANK TEST	0.00	20:02

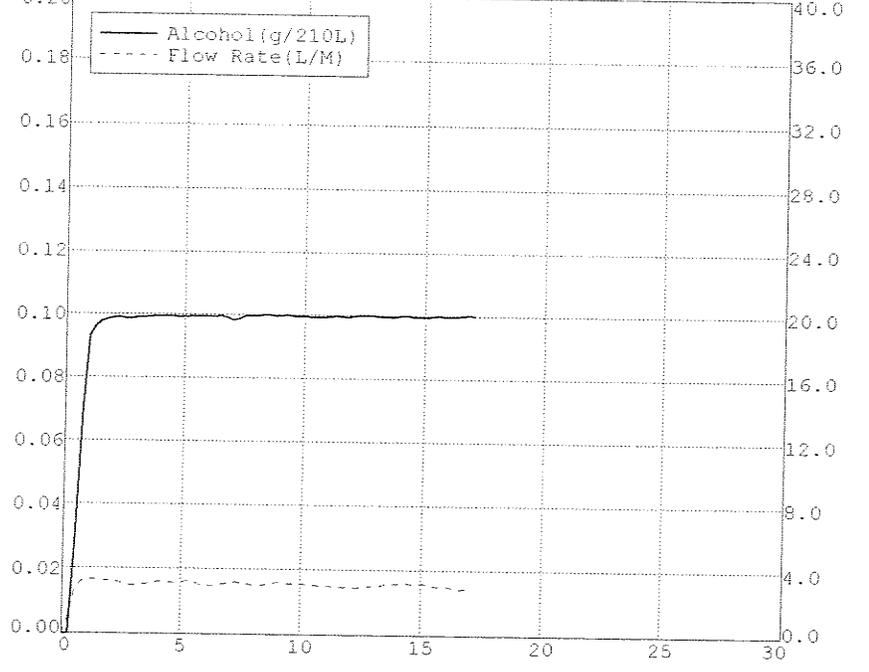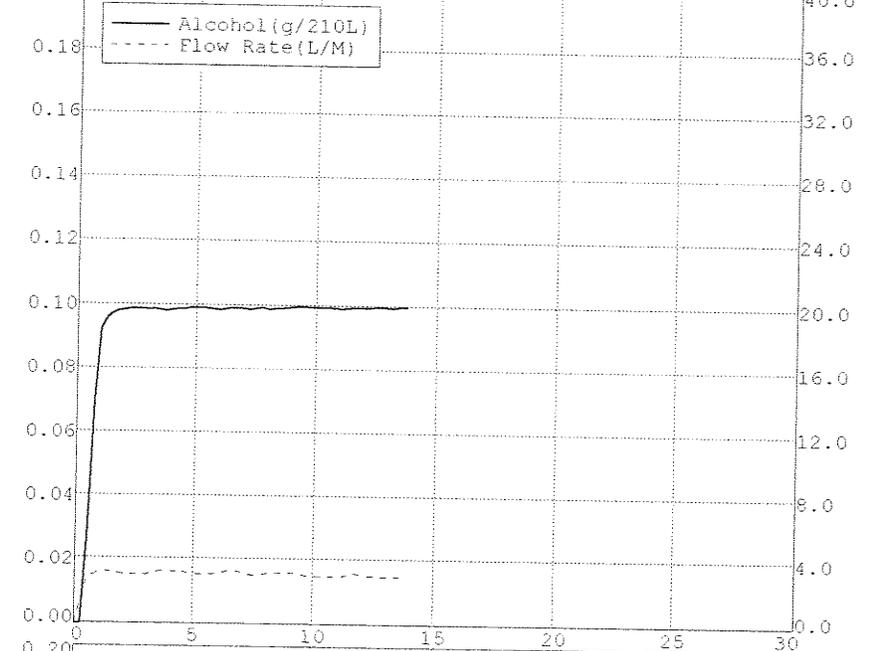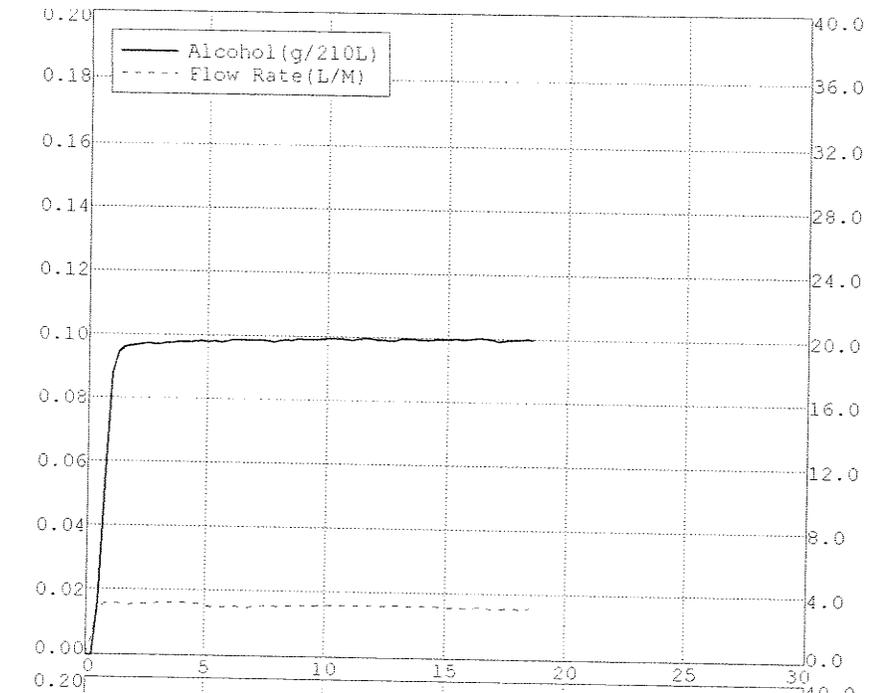

Charles B. Geisler #241