

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606

Date: 01/07/2019

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 18310

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 20:46 |
| INTERNAL STANDARD       | VERIFIED | 20:46 |
| REFERENCE STANDARD TEMP | 33.99c   |       |
| REFERENCE STANDARD      | 0.09     | 20:46 |
| BLANK TEST              | 0.00     | 20:47 |
| REFERENCE STANDARD TEMP | 33.99c   |       |
| REFERENCE STANDARD      | 0.09     | 20:47 |
| BLANK TEST              | 0.00     | 20:48 |
| REFERENCE STANDARD TEMP | 33.99c   |       |
| REFERENCE STANDARD      | 0.10     | 20:49 |
| BLANK TEST              | 0.00     | 20:49 |

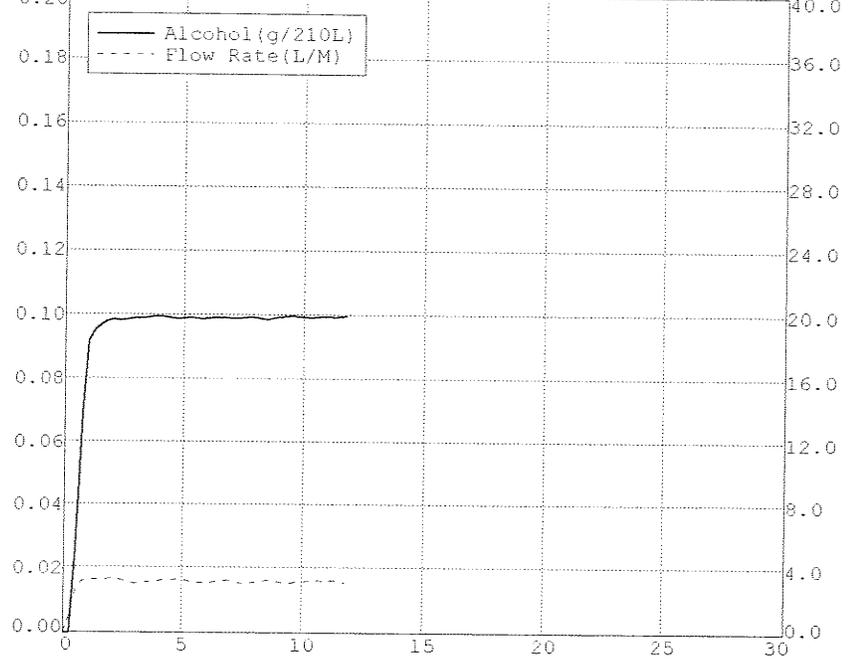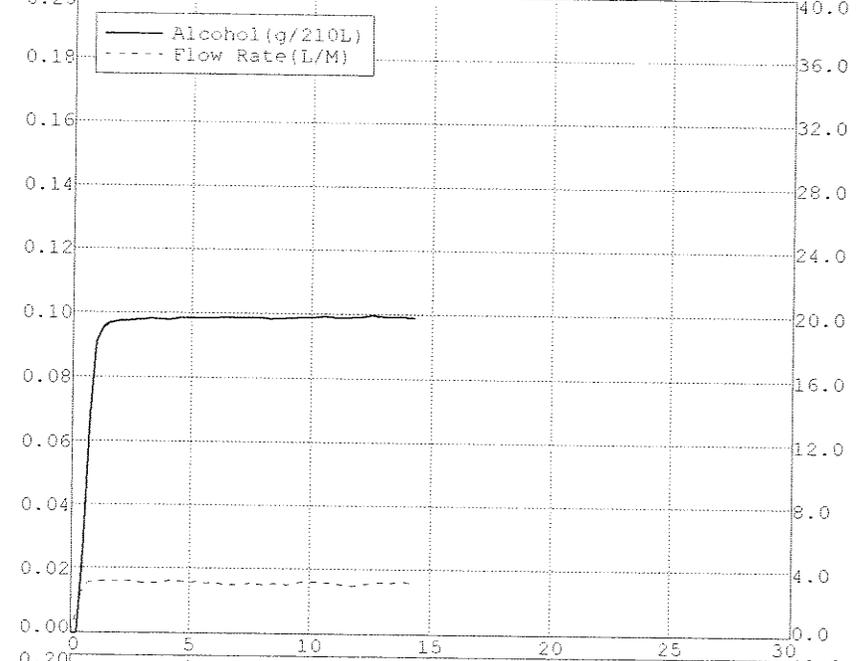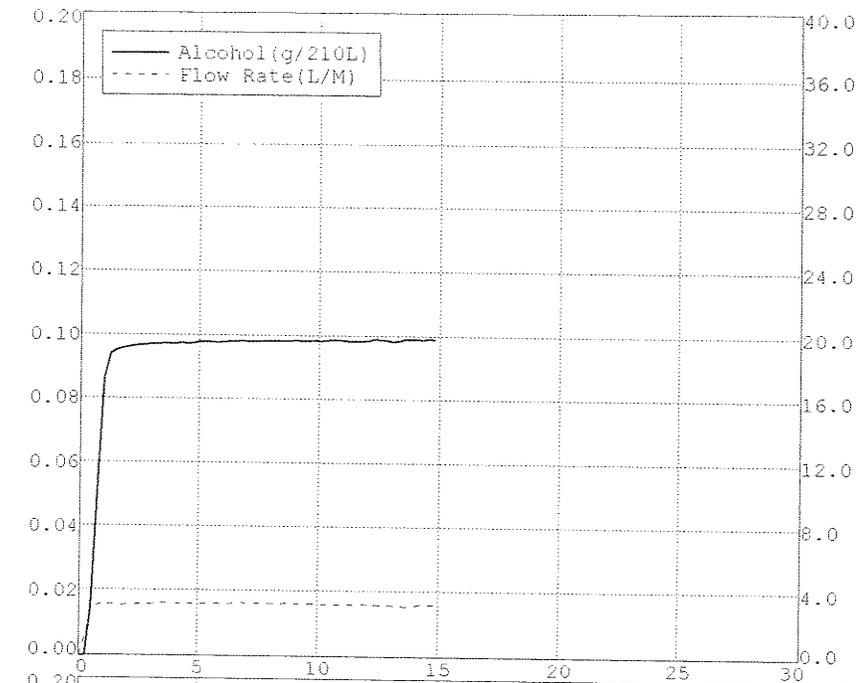

*Charles B. Geisler* #33757