

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/12/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:16
INTERNAL STANDARD	VERIFIED	20:16
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	20:17
BLANK TEST	0.00	20:18
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	20:18
BLANK TEST	0.00	20:19
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	20:19
BLANK TEST	0.00	20:20

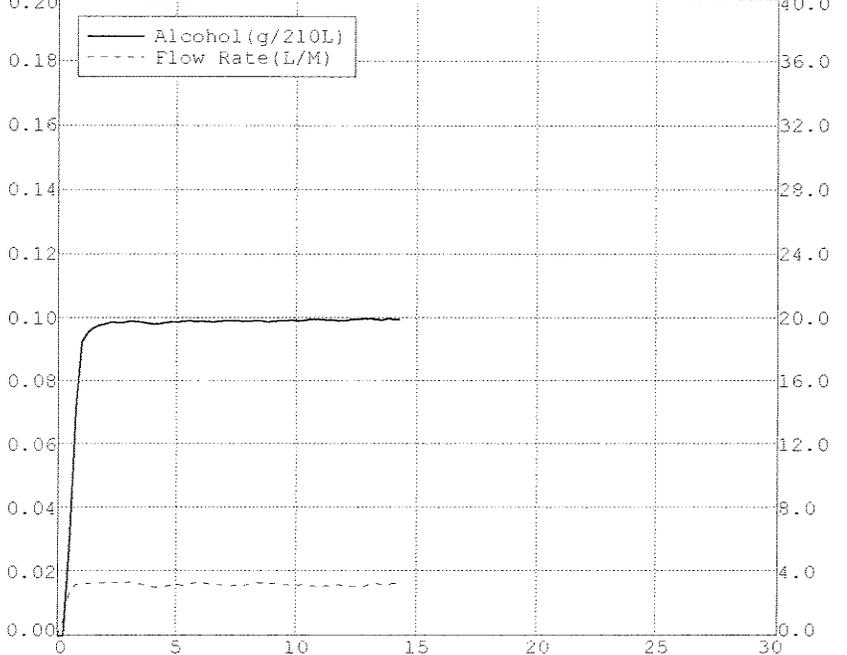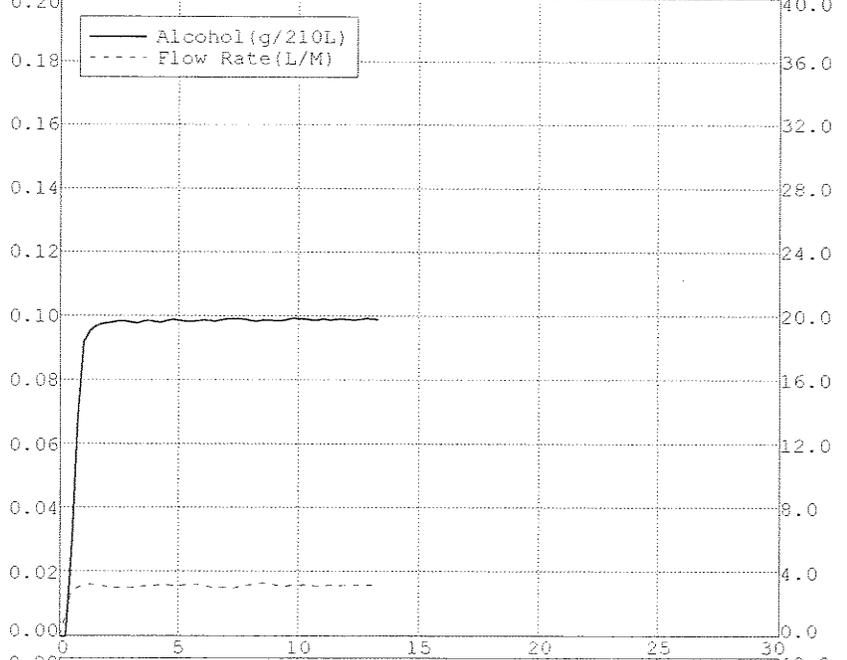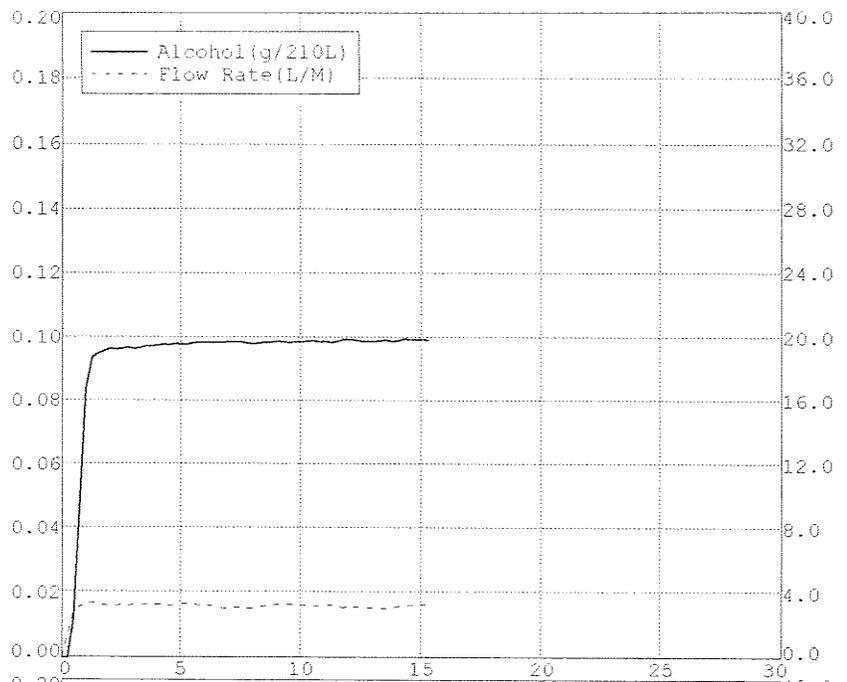

Charles B. Geisler #241