

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/27/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:27
INTERNAL STANDARD	VERIFIED	21:27
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:28
BLANK TEST	0.00	21:29
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:29
BLANK TEST	0.00	21:30
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:30
BLANK TEST	0.00	21:31

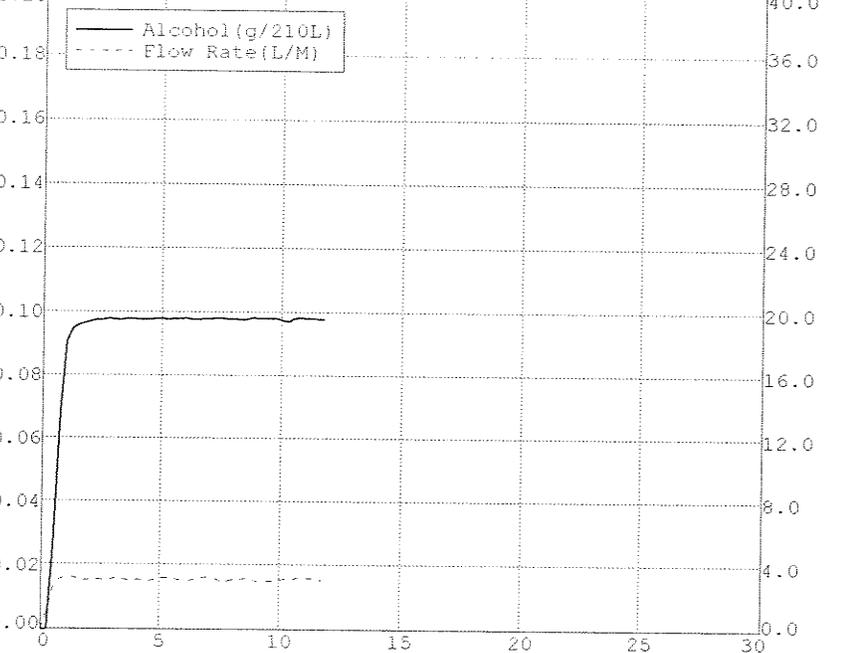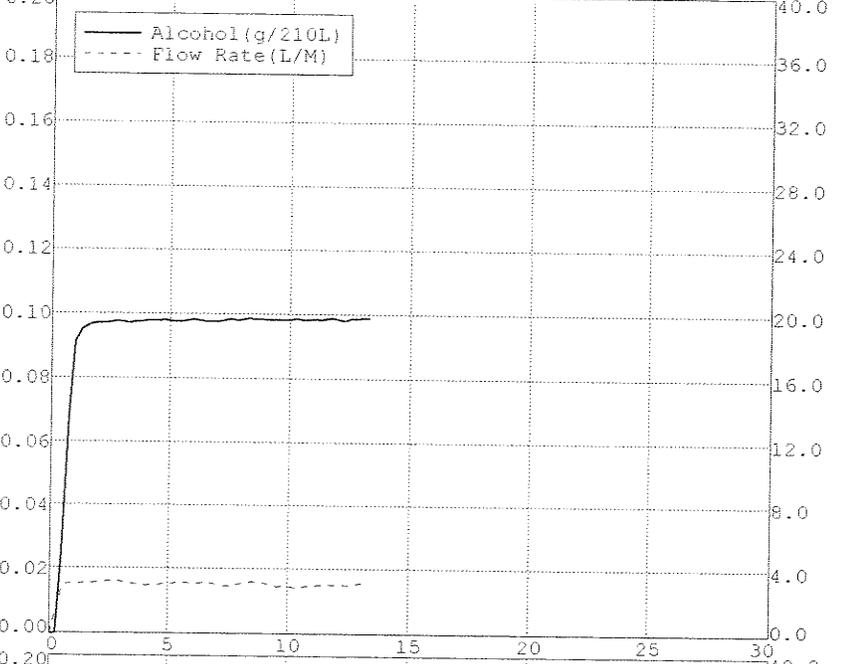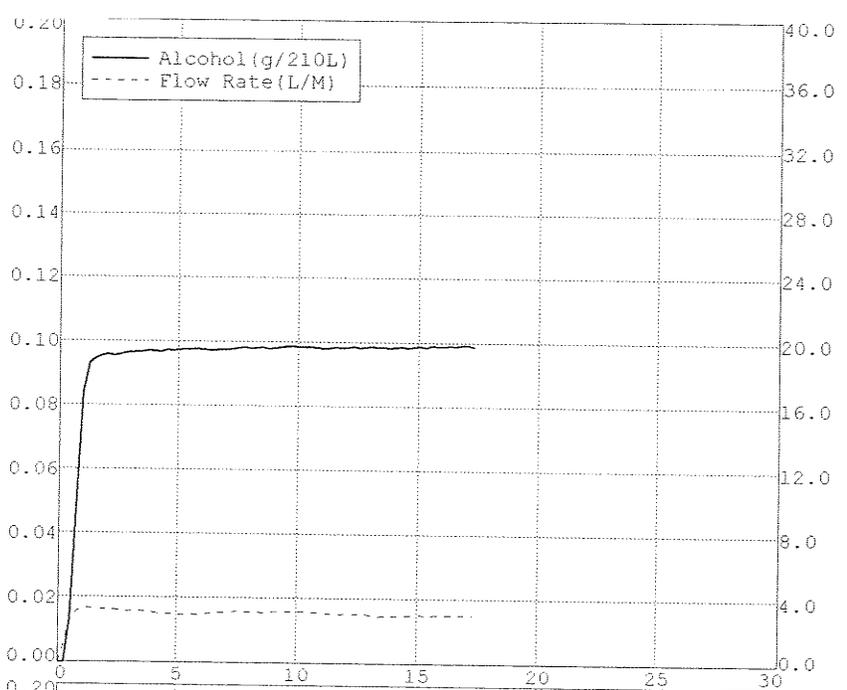

J. C. W. - 13 *[Signature]* #200