

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/01/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18360

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 02:54 |
| INTERNAL STANDARD | VERIFIED | 02:54 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.09 | 02:54 |
| BLANK TEST | 0.00 | 02:55 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.10 | 02:55 |
| BLANK TEST | 0.00 | 02:56 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.10 | 02:57 |
| BLANK TEST | 0.00 | 02:57 |

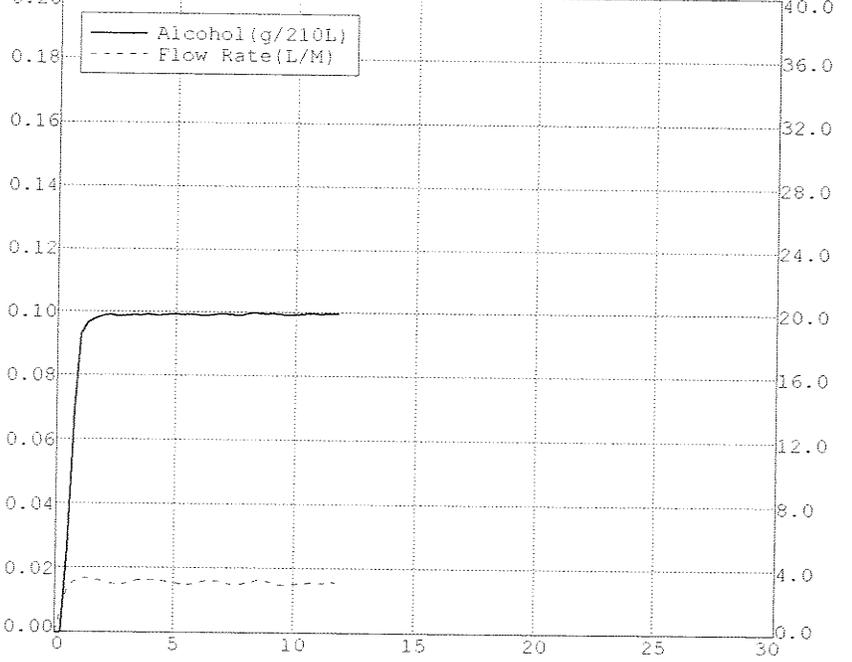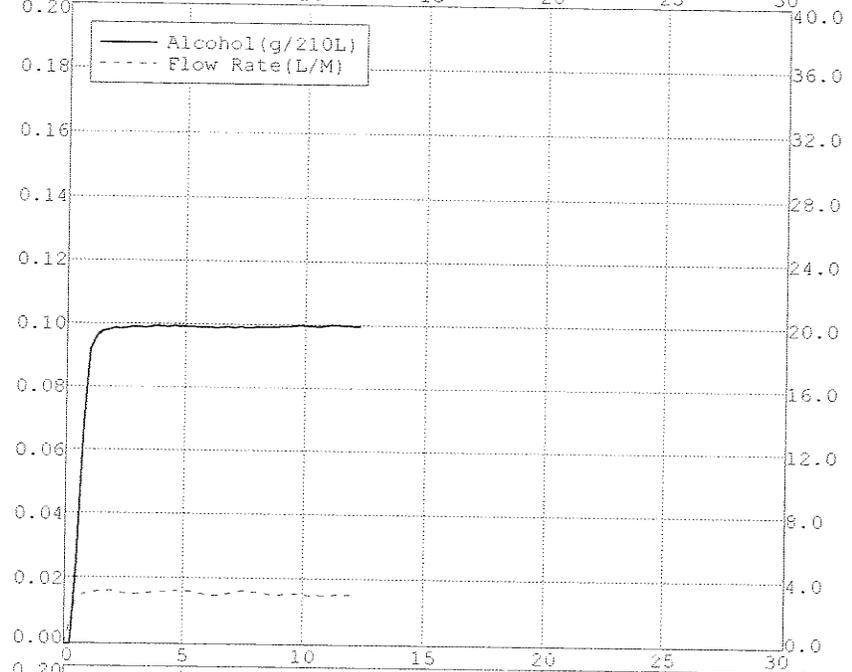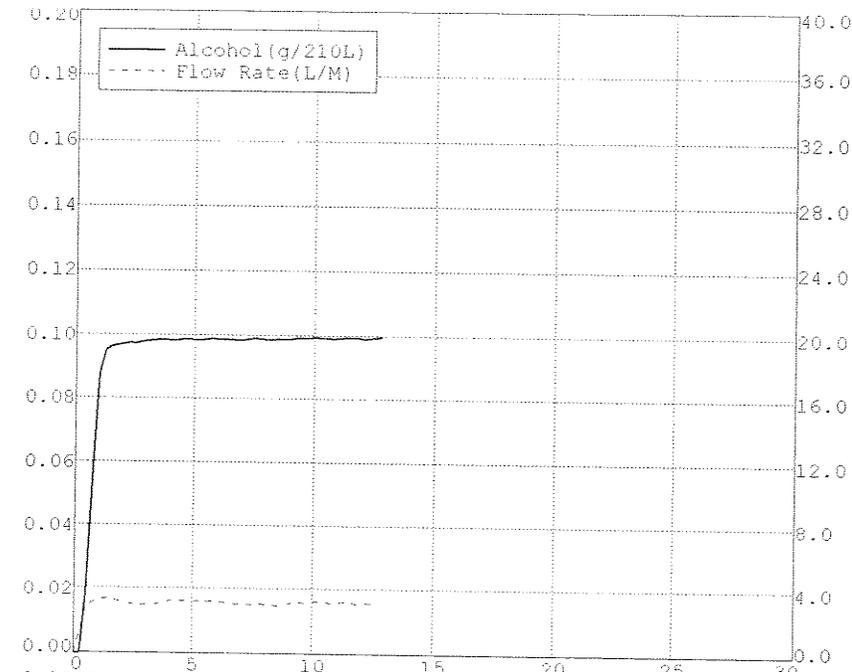

Charles B. Geisler
#33757