

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 02/04/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:03
INTERNAL STANDARD	VERIFIED	21:03
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	21:03
BLANK TEST	0.00	21:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:04
BLANK TEST	0.00	21:05
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	21:06
BLANK TEST	0.00	21:07

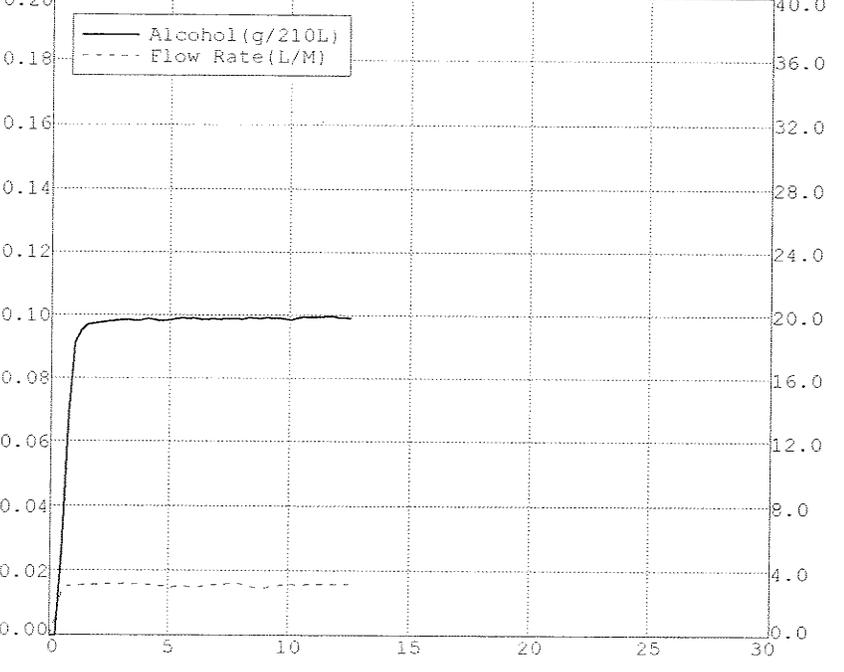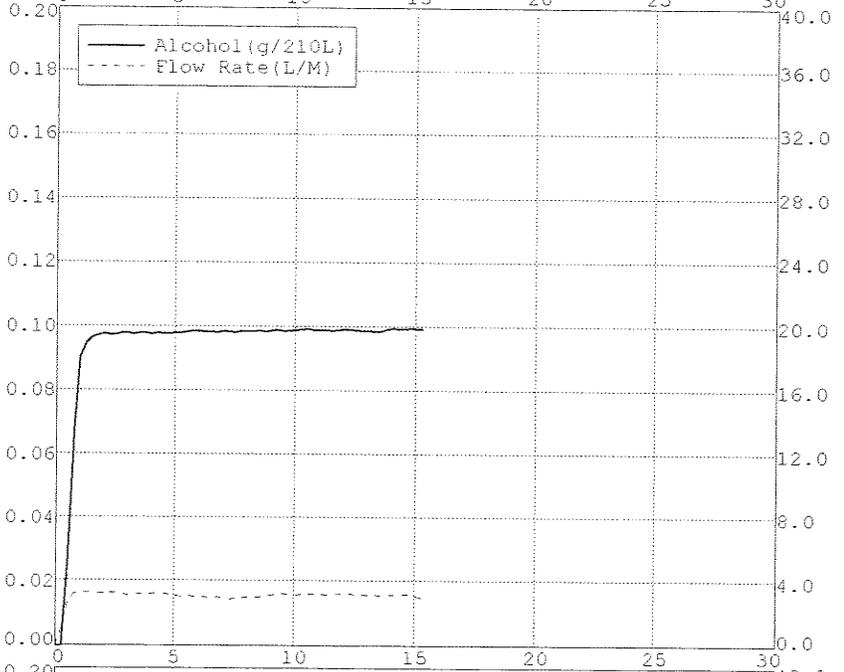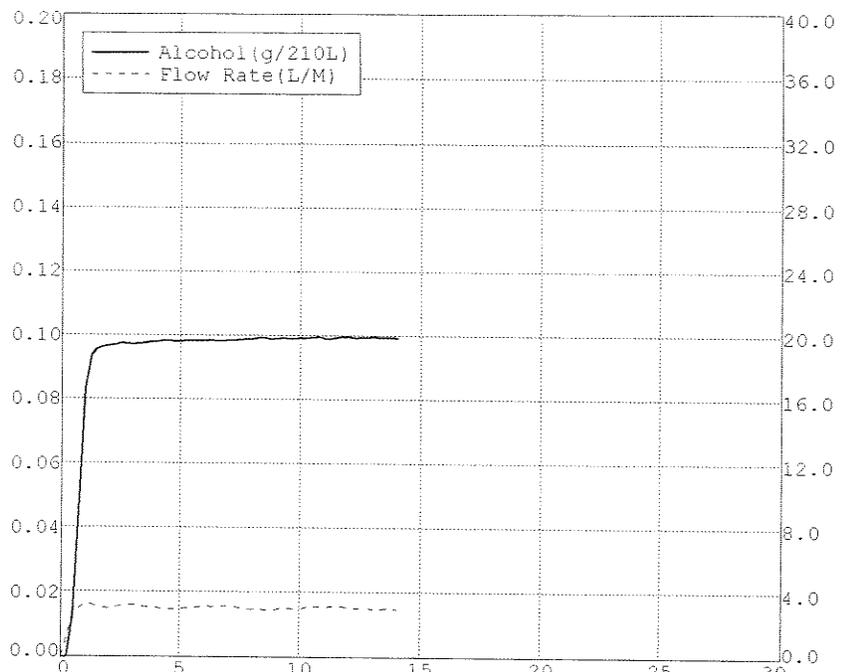

*Charles B. Geisler* #200