

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 02/19/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:46
INTERNAL STANDARD	VERIFIED	00:46
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	00:46
BLANK TEST	0.00	00:47
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:47
BLANK TEST	0.00	00:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:49
BLANK TEST	0.00	00:49

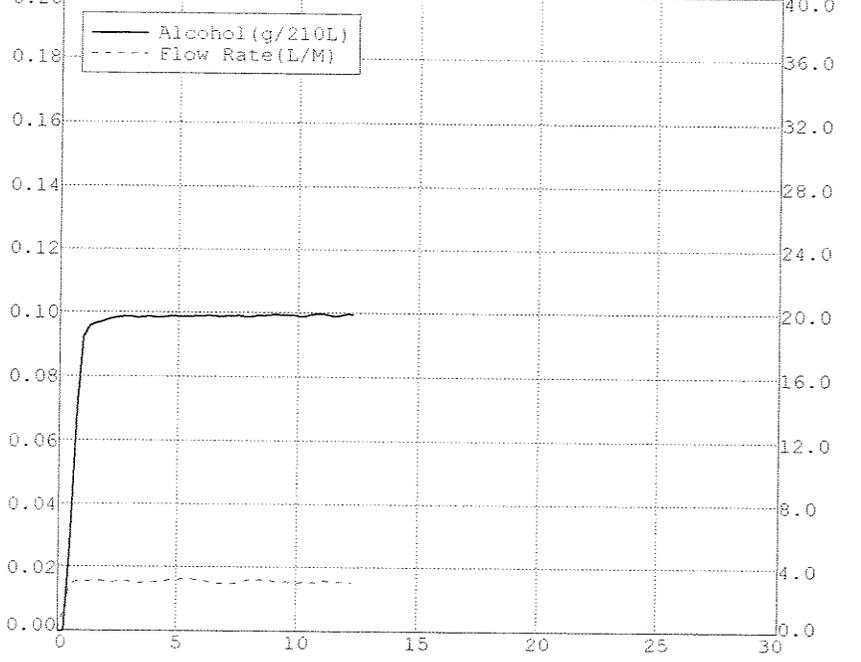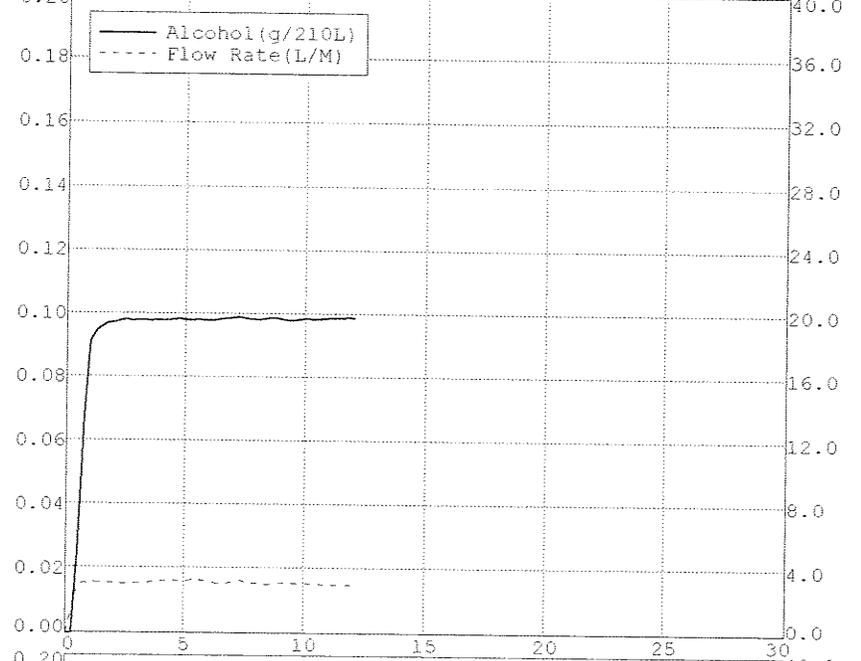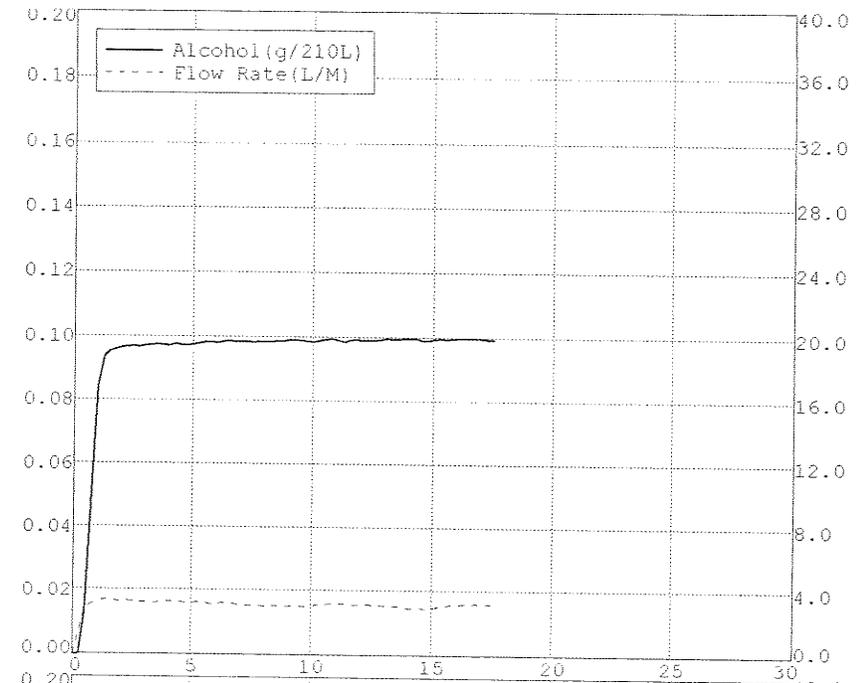

*Charles B. Geisler* #2018