

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/24/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:11
INTERNAL STANDARD	VERIFIED	21:11
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:11
BLANK TEST	0.00	21:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:12
BLANK TEST	0.00	21:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:14
BLANK TEST	0.00	21:14

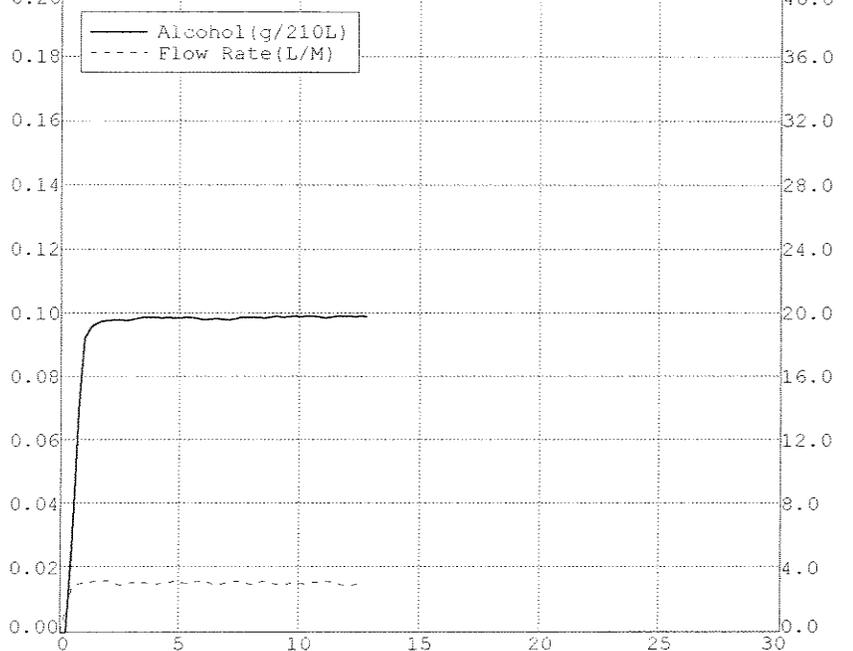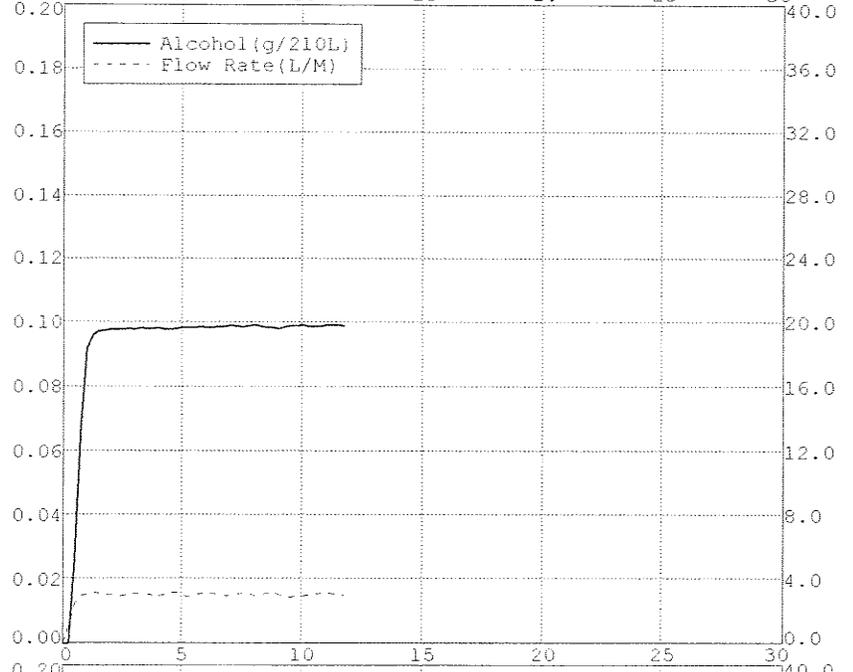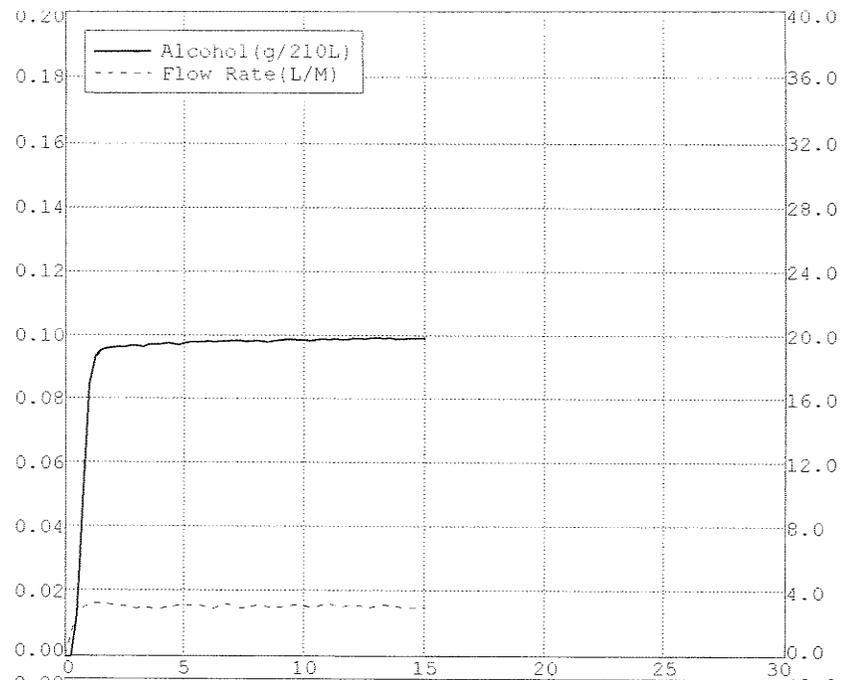

Handwritten signature: C. B. Geisler #241