

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 03/01/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:20
INTERNAL STANDARD	VERIFIED	01:20
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	01:21
BLANK TEST	0.00	01:21
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	01:22
BLANK TEST	0.00	01:23
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	01:23
BLANK TEST	0.00	01:24

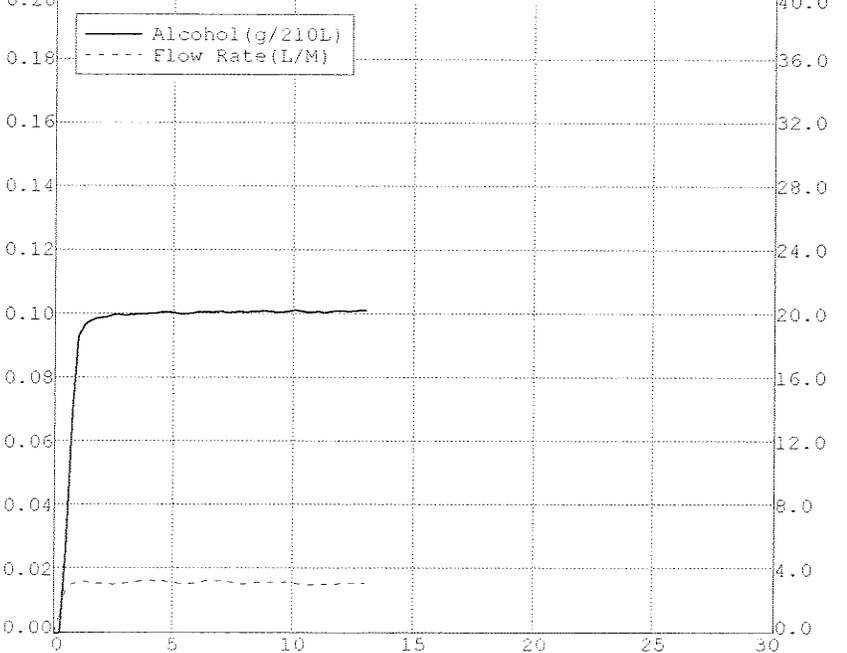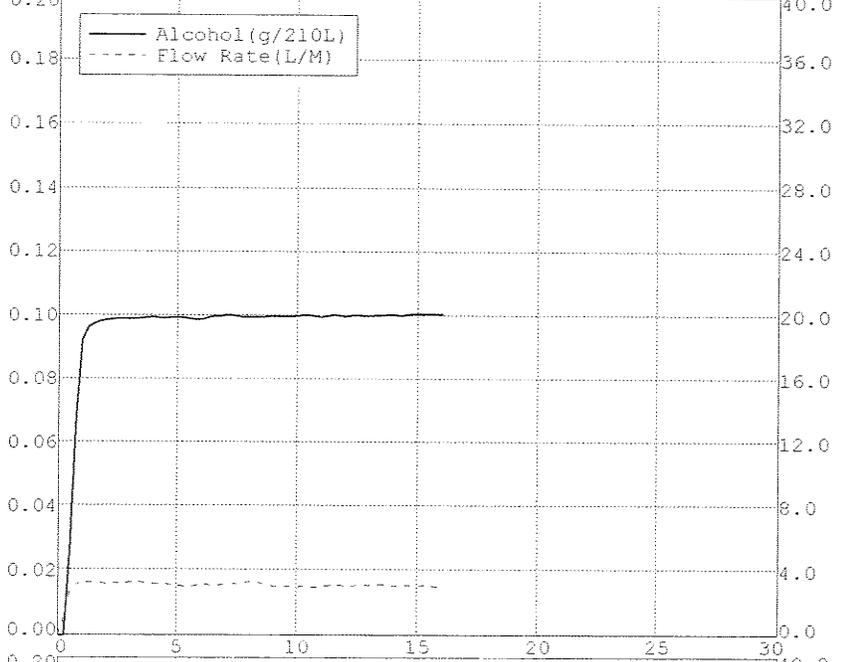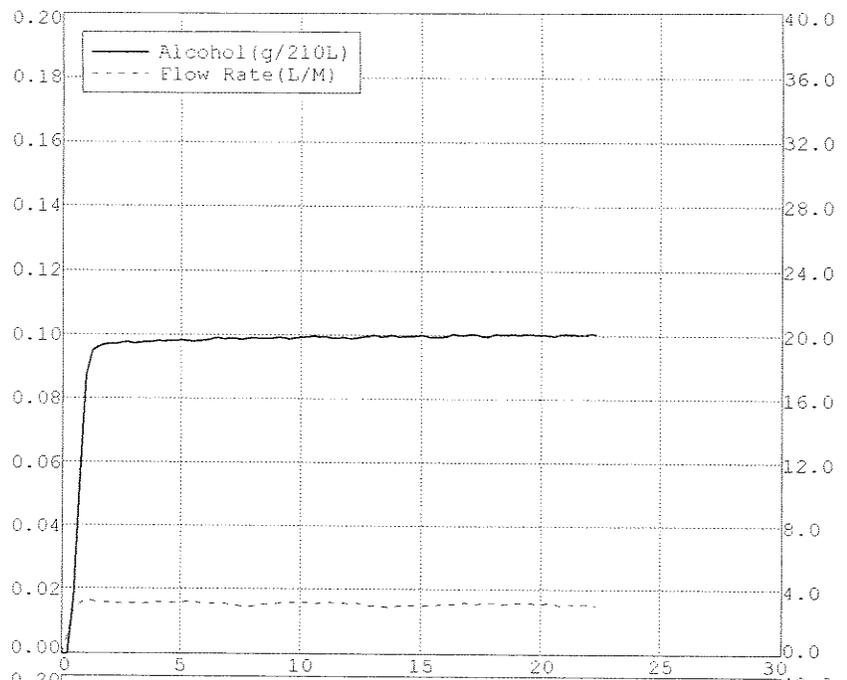

*Charles B. Geisler* #2415