

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 03/09/2019

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:25
INTERNAL STANDARD	VERIFIED	20:25
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	20:25
BLANK TEST	0.00	20:26
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	20:26
BLANK TEST	0.00	20:27
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	20:28
BLANK TEST	0.00	20:29

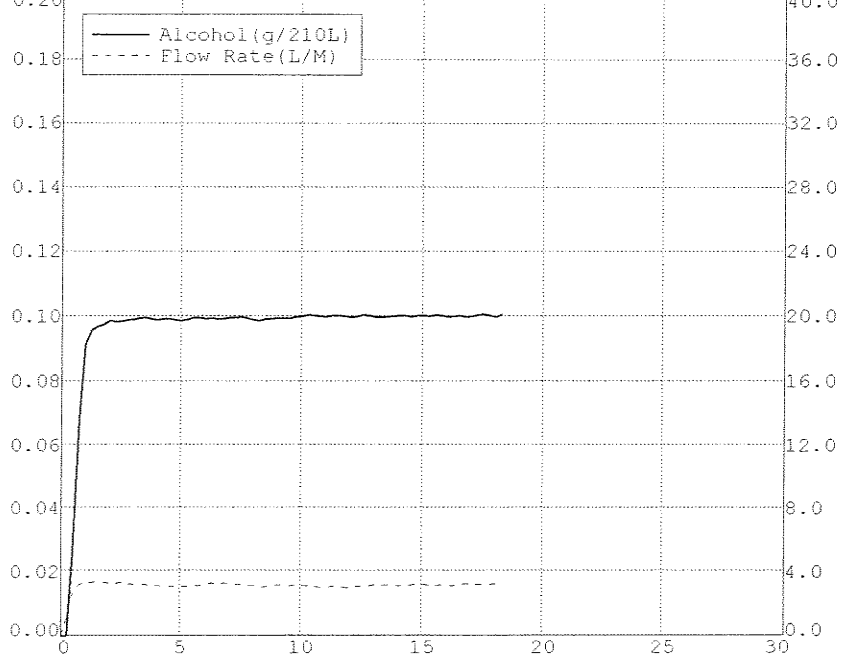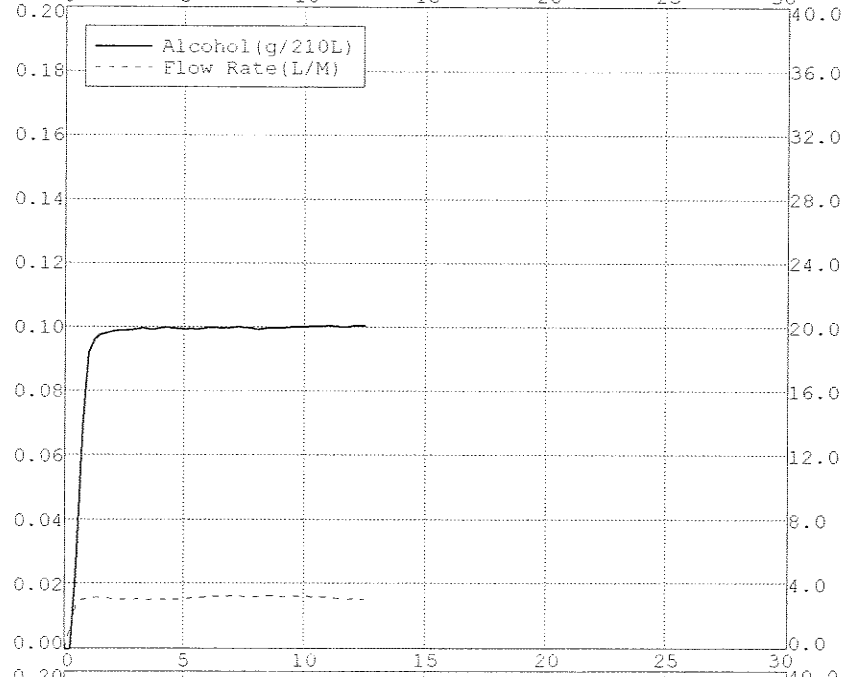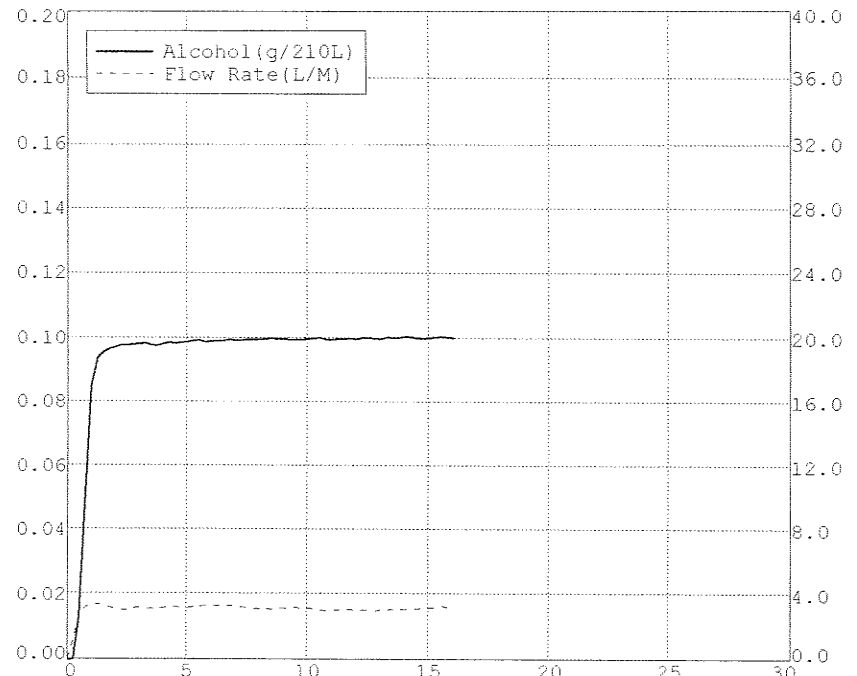

Handwritten signature: C. B. Geisler #24