

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 03/22/2019

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18360

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:33
INTERNAL STANDARD	VERIFIED	22:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:34
BLANK TEST	0.00	22:35
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	22:35
BLANK TEST	0.00	22:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:36
BLANK TEST	0.00	22:37

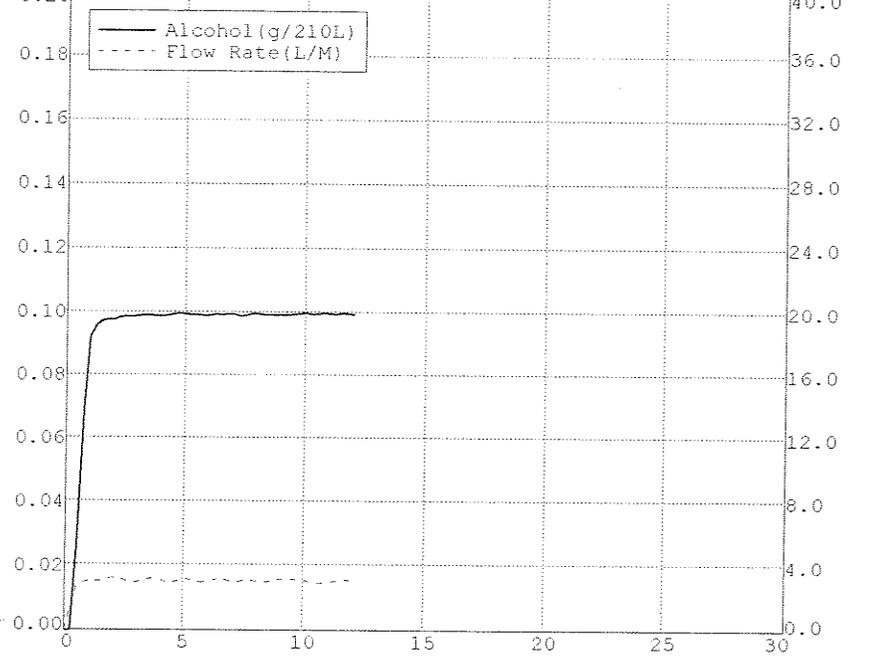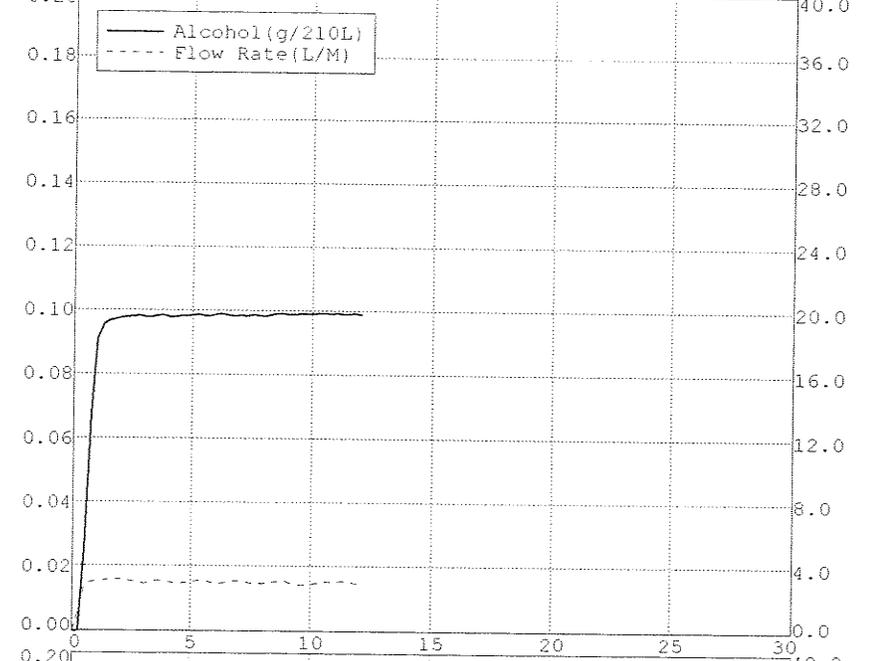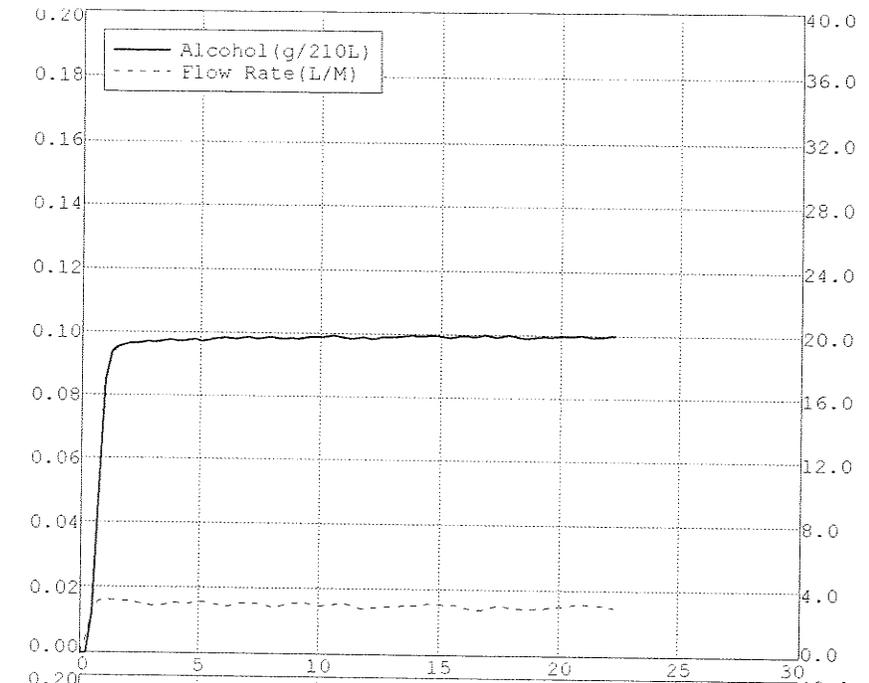

*Handwritten signature: C. B. Geisler*